

Sample Name :RGD
 Cat No. :RP20297
 Lot No. :E8502920E
 Time Processed :15:53:58
 Month-Day-Year Processed :05/19/20

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

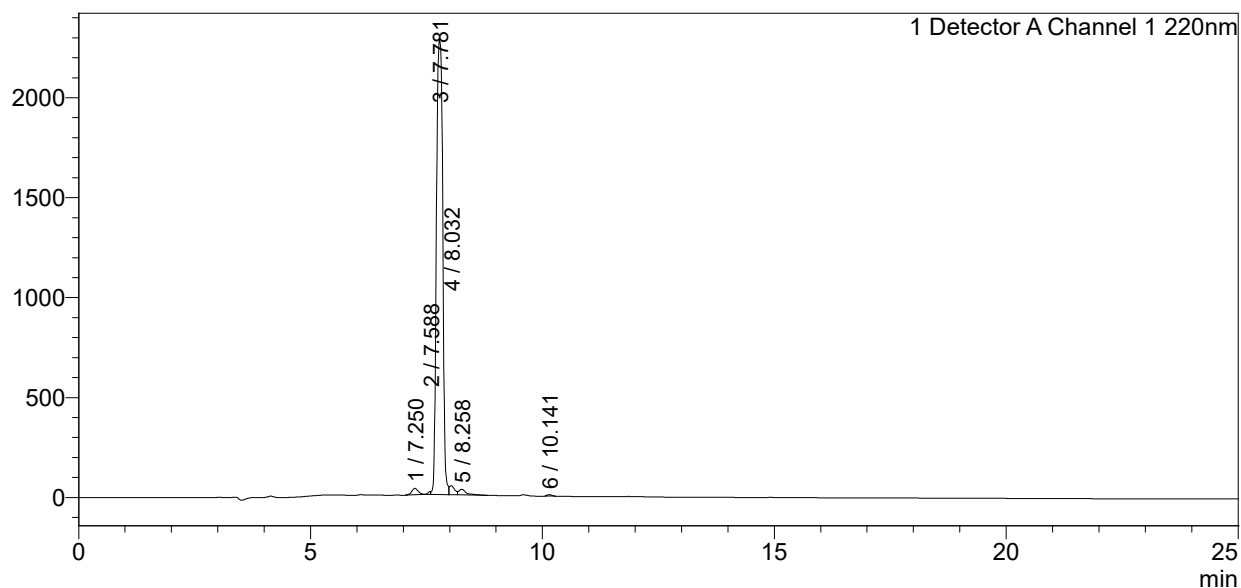

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.250	305114	31970	1.361
2	7.588	59444	14961	0.265
3	7.781	21326944	2279067	95.154
4	8.032	356352	44605	1.590
5	8.258	317073	27997	1.415
6	10.141	48187	7282	0.215
Total		22413115	2405883	100.000