

Sample Name : Biotin-TAT (47-57)
 Cat. No. : RP20408
 Lot. No.: PE8851902
 Time Processed :17:40:45
 Month-Day-Year Processed :03/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

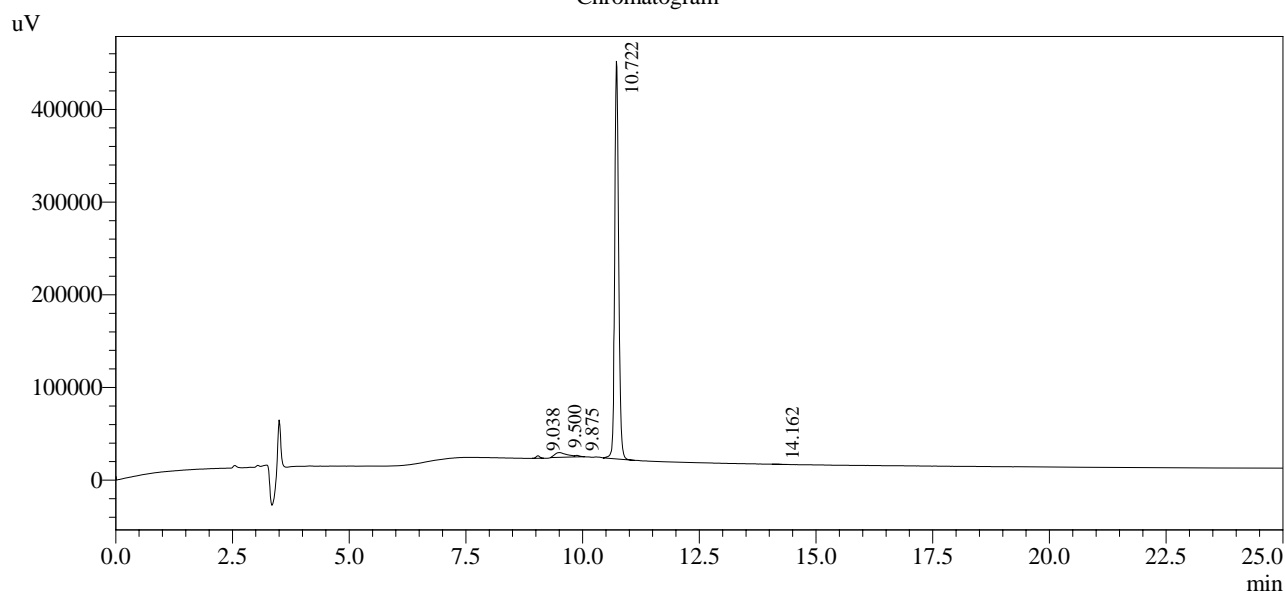

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.038	14998	2696	0.564
2	9.500	91363	5061	3.439
3	9.875	10722	1592	0.404
4	10.722	2537515	429059	95.510
5	14.162	2218	243	0.083
Total		2656816	438652	100.000