

Sample Name :InsB 9-23
 Cat. No. : RP20391
 Lot. No. : E4949219I
 Time Processed :7:55:50
 Month-Day-Year Processed : 09/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

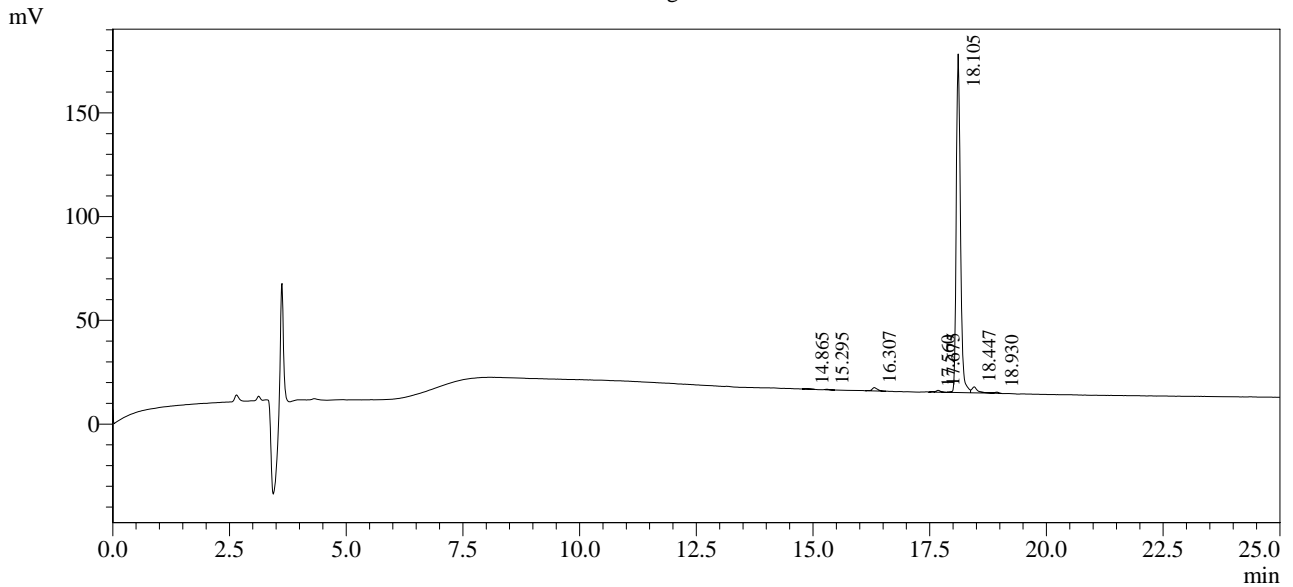

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.865	1403	188	0.131
2	15.295	1364	264	0.127
3	16.307	12899	1620	1.202
4	17.560	1939	359	0.181
5	17.675	6093	905	0.568
6	18.105	1021038	163204	95.133
7	18.447	25283	2882	2.356
8	18.930	3257	539	0.303
Total		1073275	169961	100.000