

Sample Name :Colivelin
 Cat No. :RP20167
 Lot No. :E5724519K
 Time Processed :14:42:41
 Month-Day-Year Processed :11/10/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

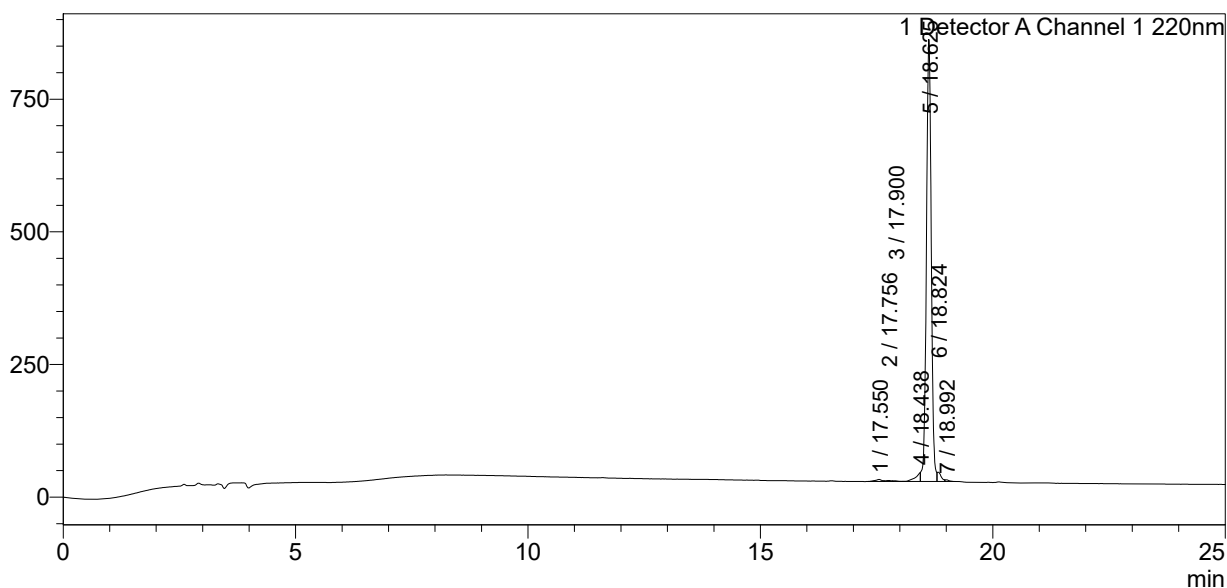

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.550	38600	3935	0.609
2	17.756	17352	1943	0.274
3	17.900	8337	1220	0.132
4	18.438	124869	16606	1.971
5	18.625	6028393	833032	95.144
6	18.824	101092	17515	1.596
7	18.992	17418	3149	0.275
Total		6336061	877400	100.000