

Sample Name :β-Amyloid Protein Precursor 770 (135-155)
 Cat No. :RP20196
 Lot No. :E4856419I
 Time Processed :23:55:24
 Month-Day-Year Processed :10/06/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

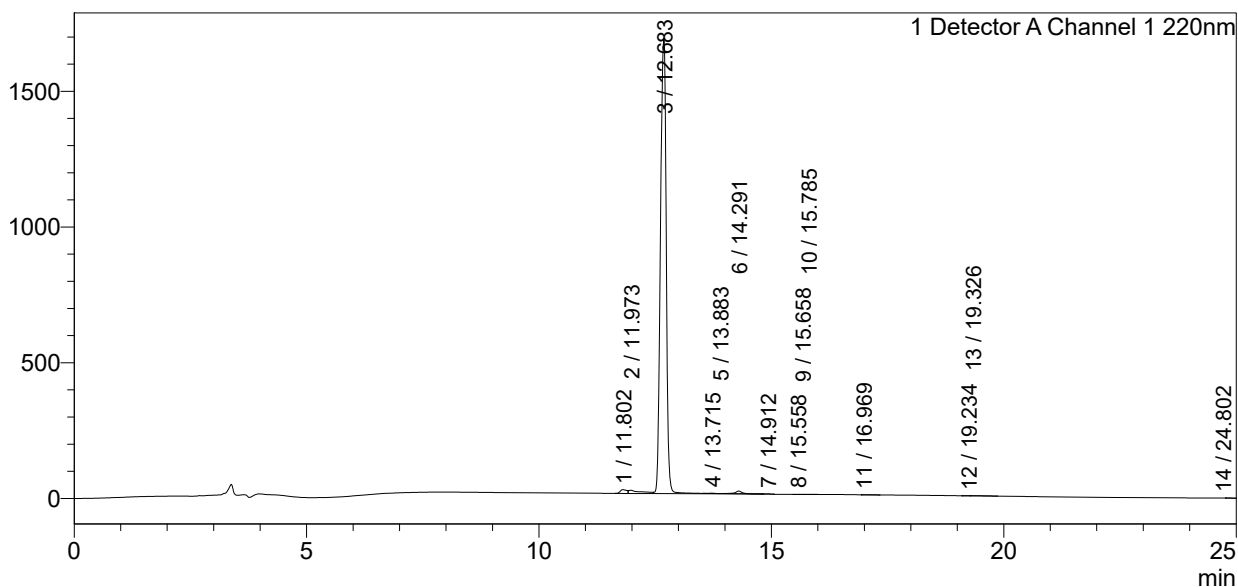

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.802	139505	14094	0.926
2	11.973	233628	12024	1.551
3	12.683	14530766	1676557	96.467
4	13.715	9376	1167	0.062
5	13.883	1974	453	0.013
6	14.291	114727	10045	0.762
7	14.912	6867	1207	0.046
8	15.558	2024	304	0.013
9	15.658	2050	405	0.014
10	15.785	7859	495	0.052
11	16.969	1272	70	0.008
12	19.234	2033	294	0.013
13	19.326	9630	465	0.064
14	24.802	1263	86	0.008
Total		15062974	1717665	100.000