

Sample Name :PUMA BH3
 Cat. No. : RP20510
 Lot. No. : E5595419J
 Time Processed :18:48:45
 Month-Day-Year Processed :11/04/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

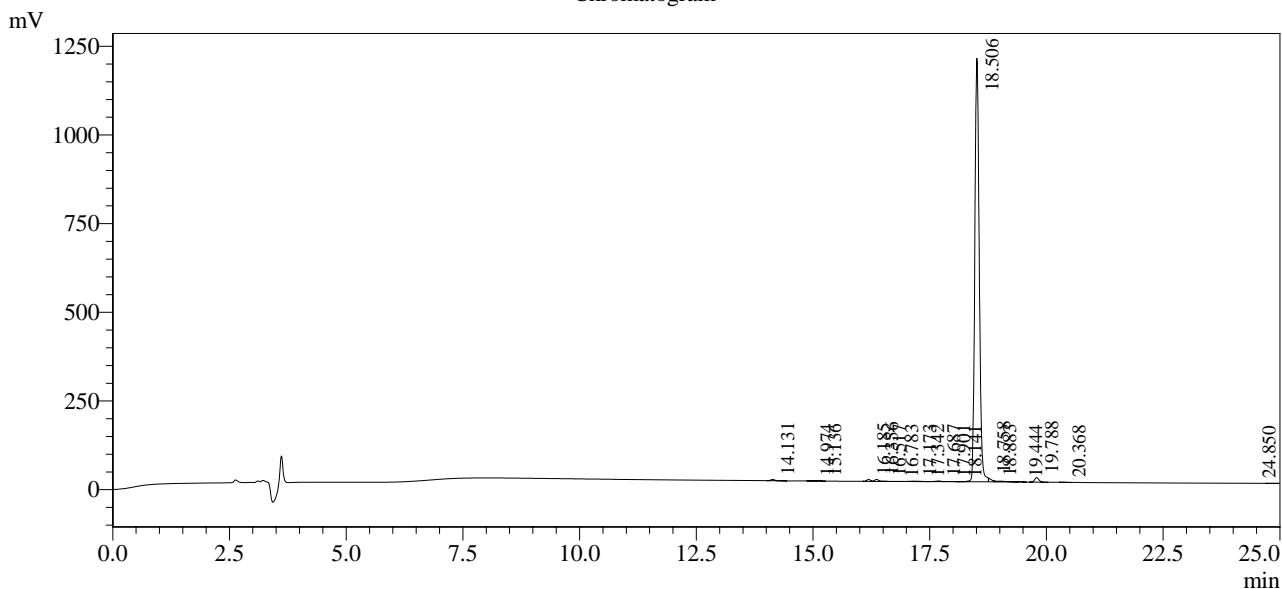

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.131	24279	4151	0.295
2	14.974	7323	1298	0.089
3	15.136	7206	1321	0.088
4	16.185	31590	5399	0.384
5	16.356	35324	5598	0.430
6	16.517	6626	1002	0.081
7	16.783	1339	285	0.016
8	17.173	17732	1669	0.216
9	17.342	2108	372	0.026
10	17.687	18352	2079	0.223
11	17.901	2921	437	0.036
12	18.141	1165	232	0.014
13	18.506	7897130	1194112	96.031
14	18.758	42558	10785	0.518
15	18.883	34718	2715	0.422
16	19.444	6132	1151	0.075
17	19.788	80329	12872	0.977
18	20.368	1487	219	0.018
19	24.850	5187	613	0.063
Total		8223505	1246309	100.000