

Sample Name :C-Peptide, dog
 Cat No. : RP11115
 Lot No. :E4792819I
 Time Processed : 20:54:15
 Month-Day-Year Processed : 09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

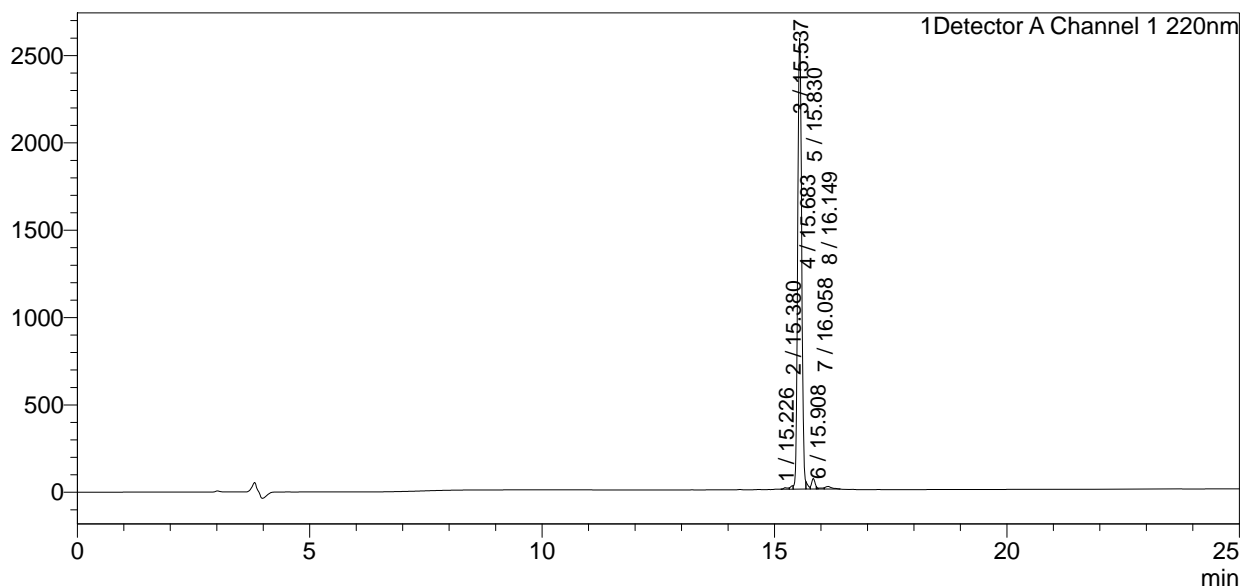

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.226	54904	8201	0.344
2	15.380	75245	18771	0.471
3	15.537	15223803	2579240	95.281
4	15.683	116394	37842	0.728
5	15.830	304926	60347	1.908
6	15.908	15740	10924	0.099
7	16.058	45017	6131	0.282
8	16.149	141841	14696	0.888
Total		15977870	2736153	100.000