


Mass Spectrum

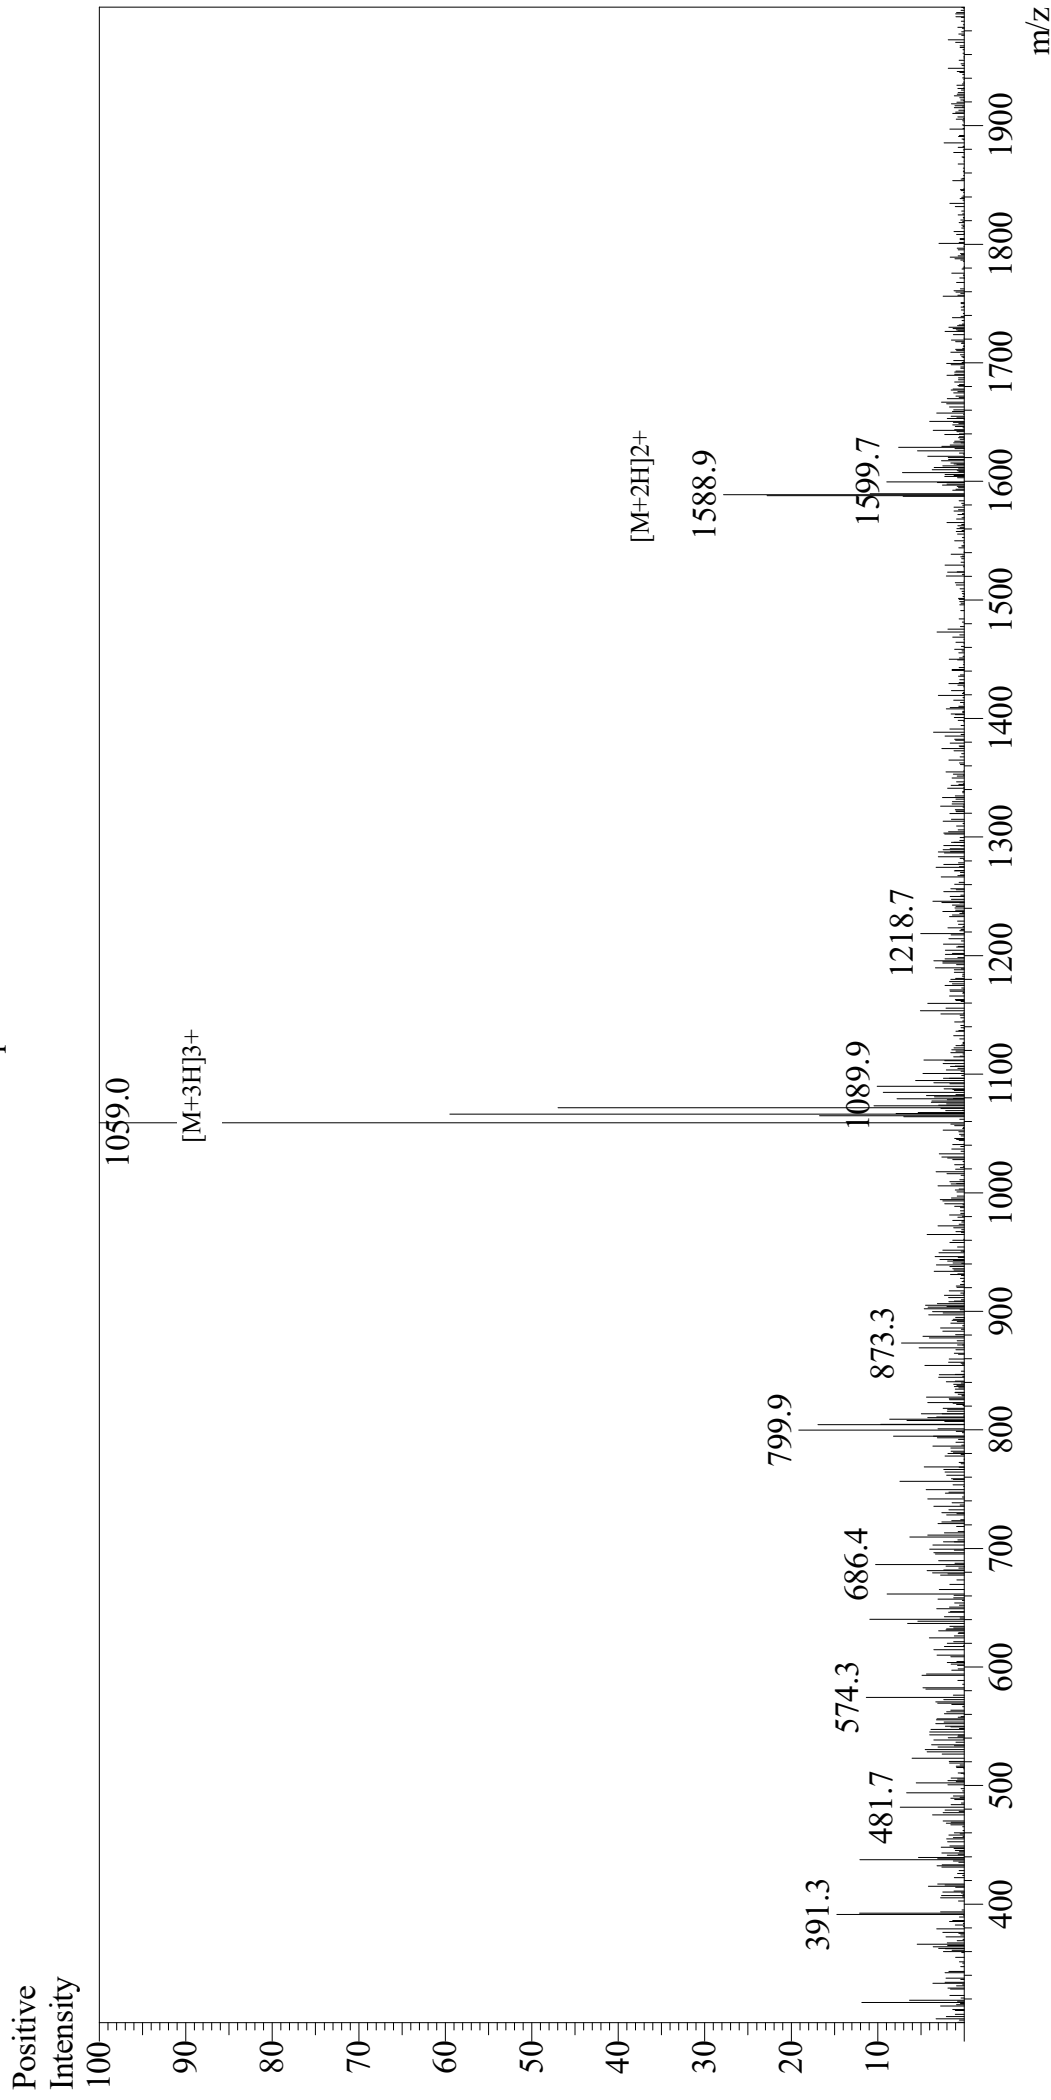

Sample Information

User : Gary
Month-Day Processed : 09/18/19
Time Processed : 02:02:49 PM
Injection Volume : 0.3
Sample Name : C-Peptide, dog
Cat No. : RP11115
Lot No. : E4792819I
Theoretical MW : 3174.49
Observed MW : 3174.0

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH