

Sample Name :Kemptide  
 Cat. No. : RP10287  
 Lot. No. : PE5821904  
 Time Processed :8:36:23

Month-Day-Year

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ17010508

### <Chromatogram>

mV

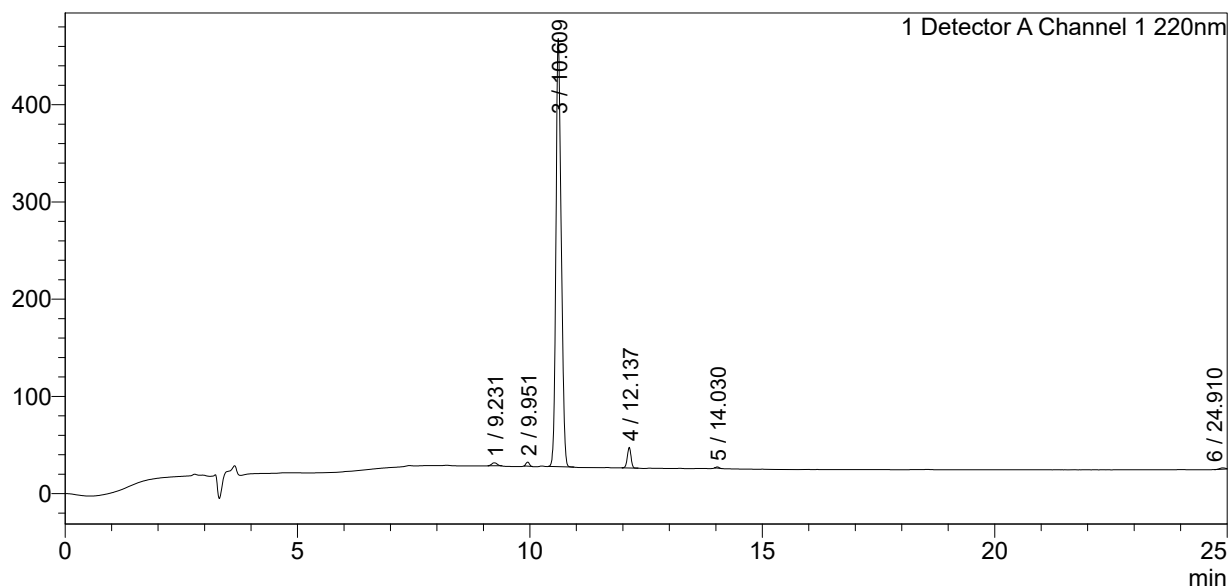

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.231	24844	3065	0.682
2	9.951	20209	4169	0.555
3	10.609	3463158	440288	95.067
4	12.137	117662	21300	3.230
5	14.030	5800	1271	0.159
6	24.910	11179	1305	0.307
Total		3642852	471398	100.000