


Mass Spectrum

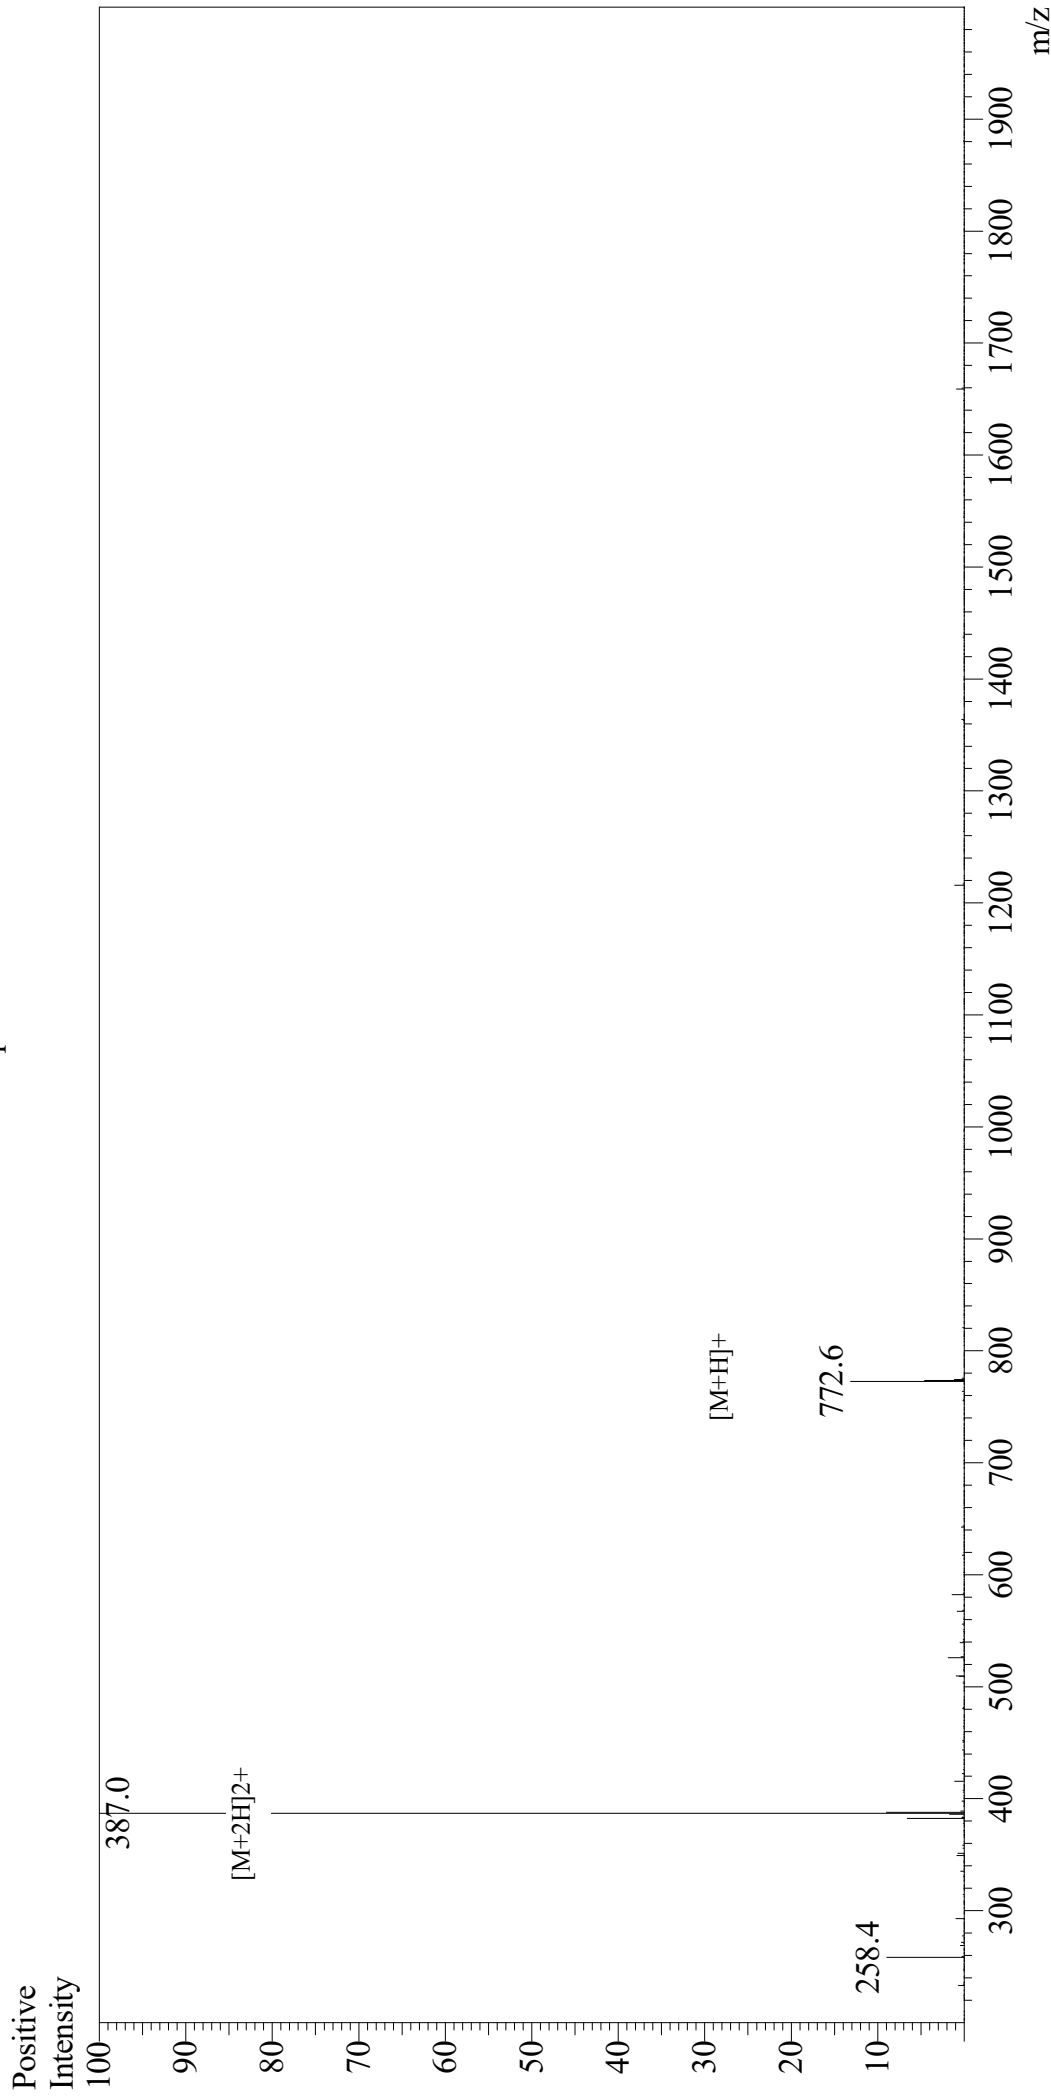

Sample Information

User : Gary
Month-Day Processed : 04/17/19
Time Processed : 11:06:34 AM
Injection Volume : 0.2
Sample Name : Kemptide
Cat No. : RP10287
Lot No. : PE5821904
Theoretical MW : 771.90
Observed MW : 772.0

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH