

Sample Name :Cardiotoxin Analog (CTX) IV (6-12)

Cat. No. : RP17303

Lot. No. : E8665320L

Time Processed :21:51:35

Month-Day-Year Processed :12/04/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ20010140

<Chromatogram>

mV

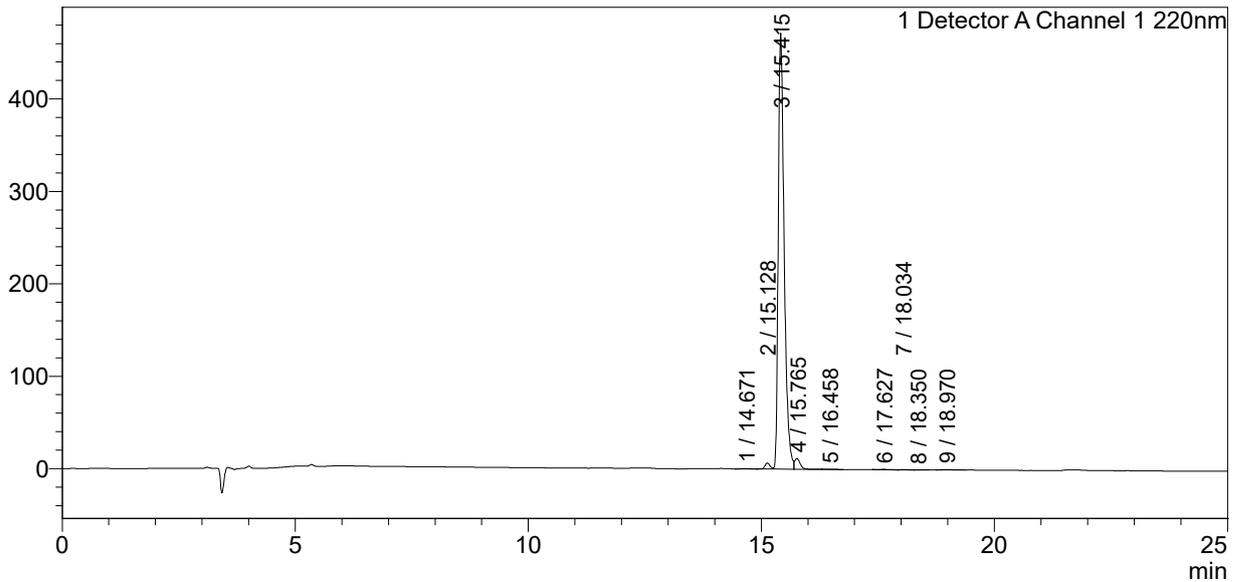

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.671	4290	329	0.099
2	15.128	49493	6530	1.146
3	15.415	4154032	471987	96.177
4	15.765	94331	11571	2.184
5	16.458	3179	304	0.074
6	17.627	4093	357	0.095
7	18.034	1647	100	0.038
8	18.350	1152	116	0.027
9	18.970	6921	531	0.160
Total		4319138	491824	100.000