

Sample Name : Angiotensin II, human
 Cat. No. : RP11257
 Lot. No. : E4657619H
 Time Processed : 0:50:15
 Month-Day-Year Processed : 08/31/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

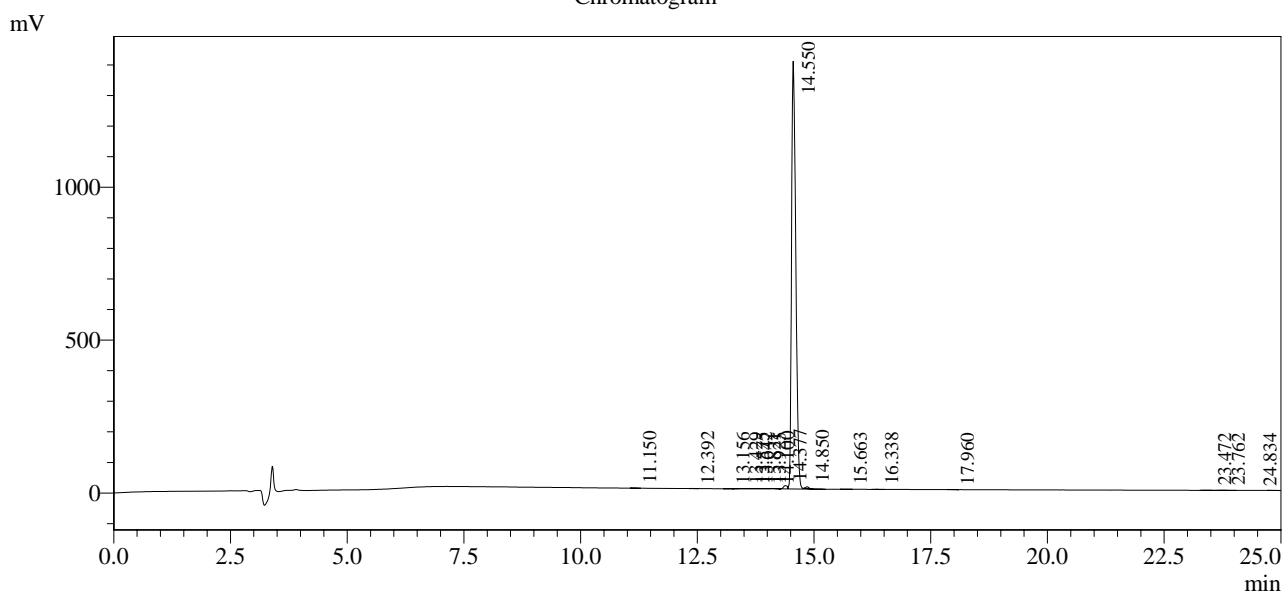

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.150	4132	803	0.046
2	12.392	1329	252	0.015
3	13.156	1384	252	0.015
4	13.429	4994	702	0.055
5	13.575	5817	803	0.064
6	13.642	6763	785	0.075
7	13.821	5583	738	0.062
8	13.925	3672	617	0.041
9	14.100	7594	1019	0.084
10	14.377	62110	10527	0.687
11	14.550	8897807	1398917	98.398
12	14.850	25641	5868	0.284
13	15.663	2346	351	0.026
14	16.338	2142	405	0.024
15	17.960	1582	271	0.017
16	23.472	2546	207	0.028
17	23.762	5481	609	0.061
18	24.834	1760	198	0.019
Total		9042683	1423323	100.000