

Sample Name :MARCKS Peptide(151-175), Phosphorylated
 Cat. No. : RP20454
 Lot. No. :E7083219J
 Time Processed :3:03:33
 Month-Day-Year Processed :10/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

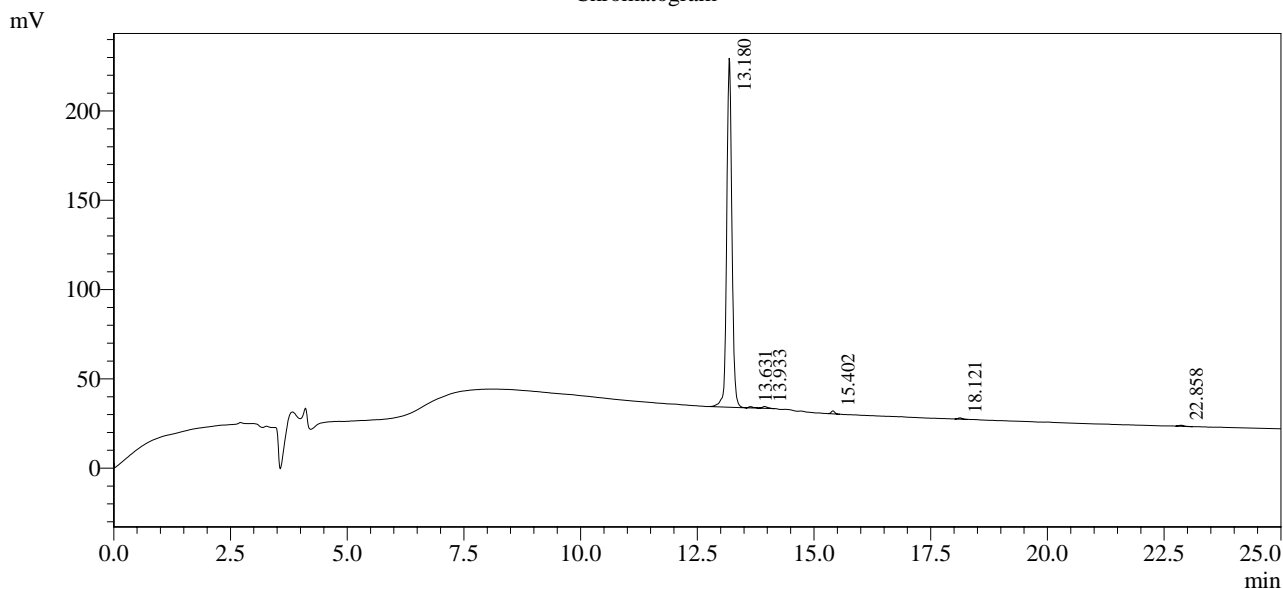

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.180	1509337	195438	97.959
2	13.631	5846	819	0.379
3	13.933	8118	1038	0.527
4	15.402	8701	1648	0.565
5	18.121	4521	732	0.293
6	22.858	4261	573	0.277
Total		1540784	200248	100.000