

Sample Name : [Des-Arg9]-Bradykinin

Cat No. : RP13625

Lot No. : E9418521D

Time Processed : 19:22:36

Month-Day-Year Processed : 04/21/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow: 1 ml/min

Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0310

<Chromatogram>

mV

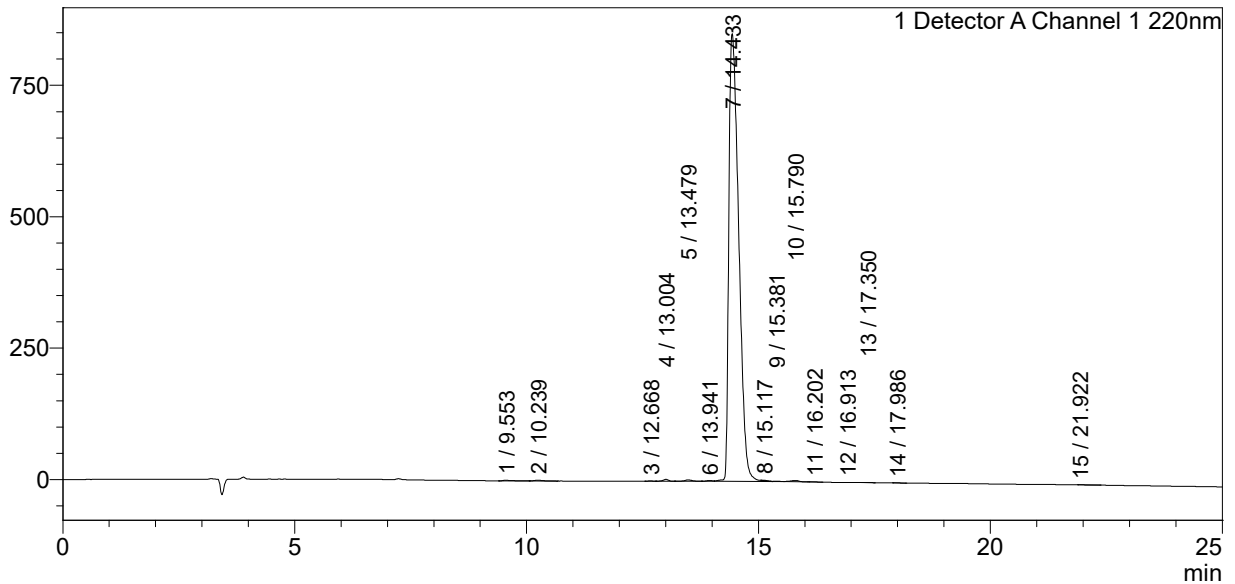

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.553	16158	1455	0.127
2	10.239	22101	1550	0.173
3	12.668	5286	731	0.041
4	13.004	32147	3723	0.252
5	13.479	34238	2731	0.268
6	13.941	15617	1474	0.122
7	14.433	12595279	852018	98.628
8	15.117	5516	848	0.043
9	15.381	4180	597	0.033
10	15.790	30318	2500	0.237
11	16.202	3152	403	0.025
12	16.913	1387	122	0.011
13	17.350	2455	361	0.019
14	17.986	1087	170	0.009
15	21.922	1560	89	0.012
Total		12770482	868773	100.000