

Sample Name :SIYRY
 Cat. No. : RP20234
 Lot. No. :E7049719J
 Time Processed :22:18:02
 Month-Day-Year Processed :10/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

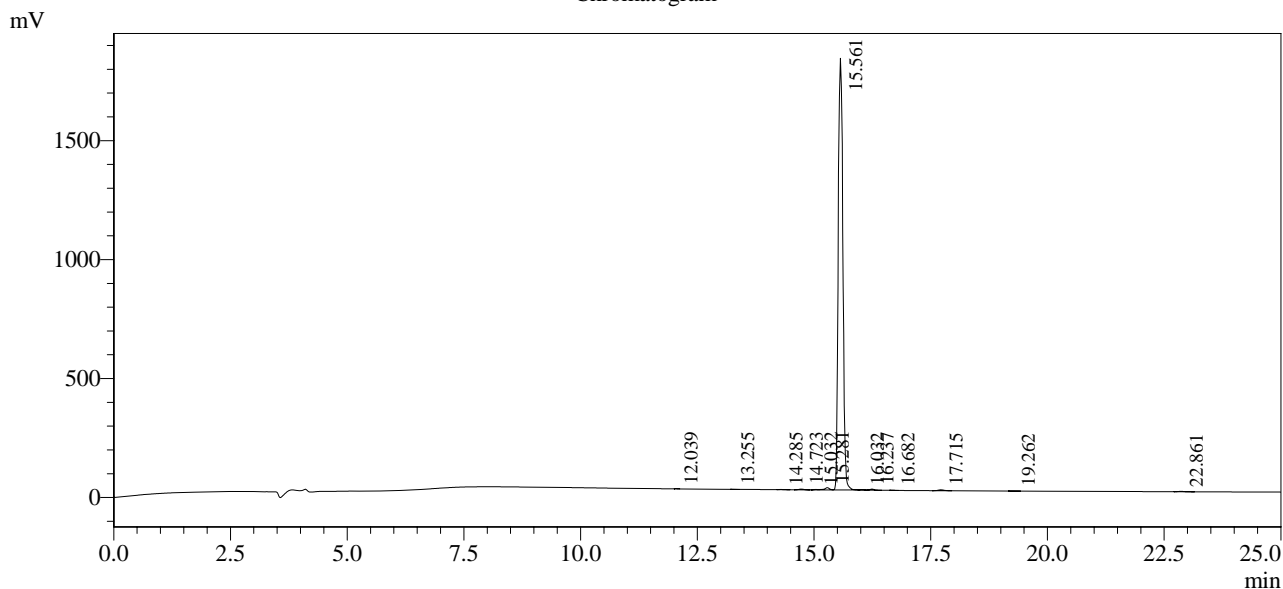

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.039	2852	1081	0.022
2	13.255	1544	344	0.012
3	14.285	5476	766	0.043
4	14.723	21891	2837	0.172
5	15.032	9322	1794	0.073
6	15.281	69711	9369	0.547
7	15.561	12559484	1814591	98.496
8	16.032	4012	742	0.031
9	16.237	23089	4259	0.181
10	16.682	2919	575	0.023
11	17.715	33129	3714	0.260
12	19.262	5330	919	0.042
13	22.861	12508	1629	0.098
Total		12751267	1842622	100.000