

Sample Name :Angiotensin II, human
 Cat No. : RP11257
 Lot No. : PE8432902
 Time Processed : 3:48:04
 Month-Day-Year Processed : 03/01/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment:GK12010012

<Chromatogram>

mV

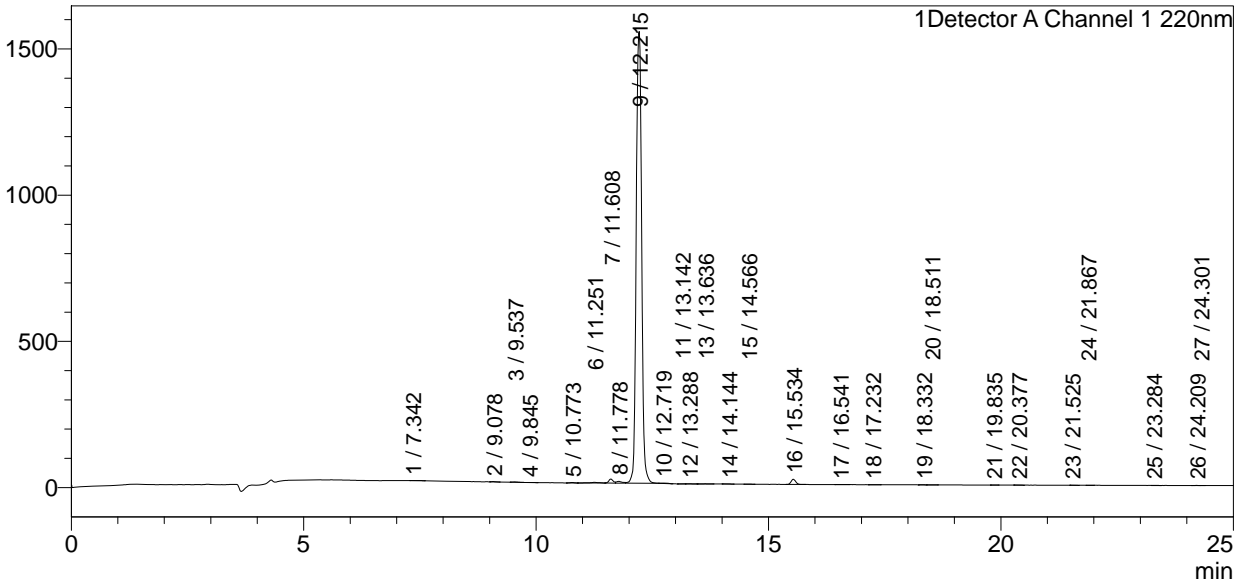

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.342	2763	295	0.022
2	9.078	6013	1162	0.047
3	9.537	10646	1257	0.083
4	9.845	2724	226	0.021
5	10.773	9322	1558	0.073
6	11.251	27789	2130	0.217
7	11.608	87864	13822	0.685
8	11.778	49241	5792	0.384
9	12.215	12451535	1544501	97.140
10	12.719	14928	1346	0.116
11	13.142	1192	250	0.009
12	13.288	3017	486	0.024
13	13.636	5052	477	0.039
14	14.144	2331	311	0.018
15	14.566	3743	557	0.029

Peak#	Ret. Time	Area	Height	Area%
16	15.534	120950	17654	0.944
17	16.541	3495	358	0.027
18	17.232	1127	110	0.009
19	18.332	1296	246	0.010
20	18.511	1122	143	0.009
21	19.835	1732	281	0.014
22	20.377	1852	276	0.014
23	21.525	1646	240	0.013
24	21.867	1485	218	0.012
25	23.284	2068	312	0.016
26	24.209	2156	313	0.017
27	24.301	1056	185	0.008
Total		12818145	1594505	100.000