

Sample Name :CLIP (86-100)
 Cat No.: RP20279
 Lot No.: E1587619I
 Time Processed :0:24:06
 Month-Day-Year Processed :09/16/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
45.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

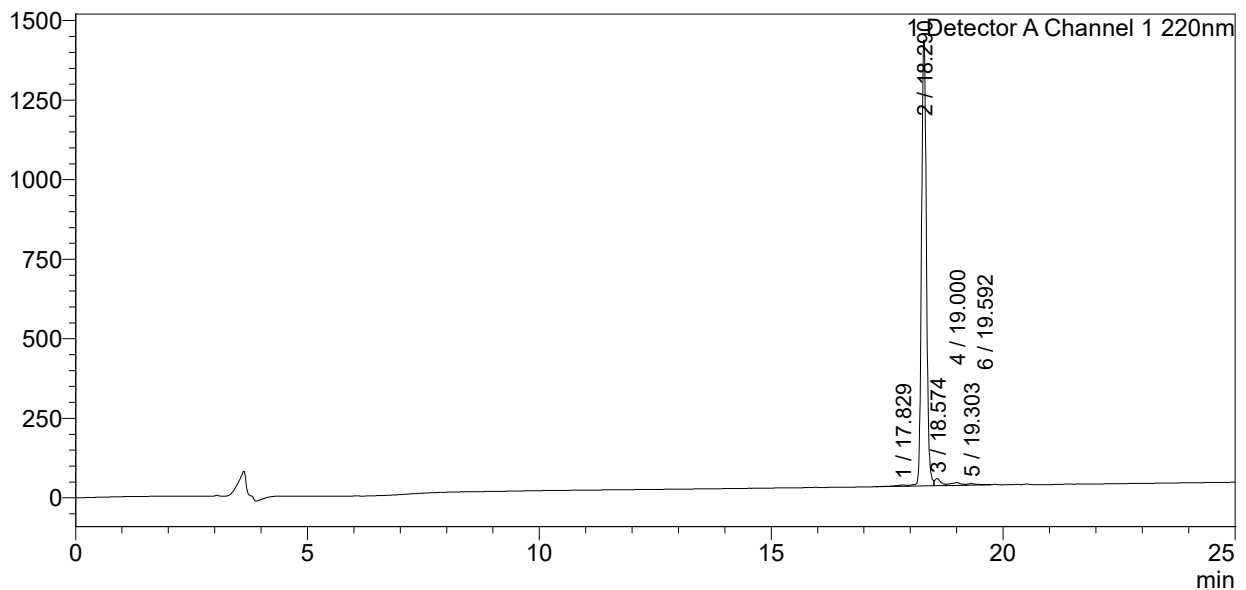

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	17.829	70198	4331	0.646
2	18.290	10372241	1401946	95.511
3	18.574	199189	22605	1.834
4	19.000	145952	8768	1.344
5	19.303	70570	5333	0.650
6	19.592	1638	340	0.015
Total		10859787	1443323	100.000