

Sample Name :Substance P, Free Acid
 Cat No.: RP10185
 Lot No.: E7251320B
 Time Processed :21:33:01
 Month-Day-Year Processed :02/05/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

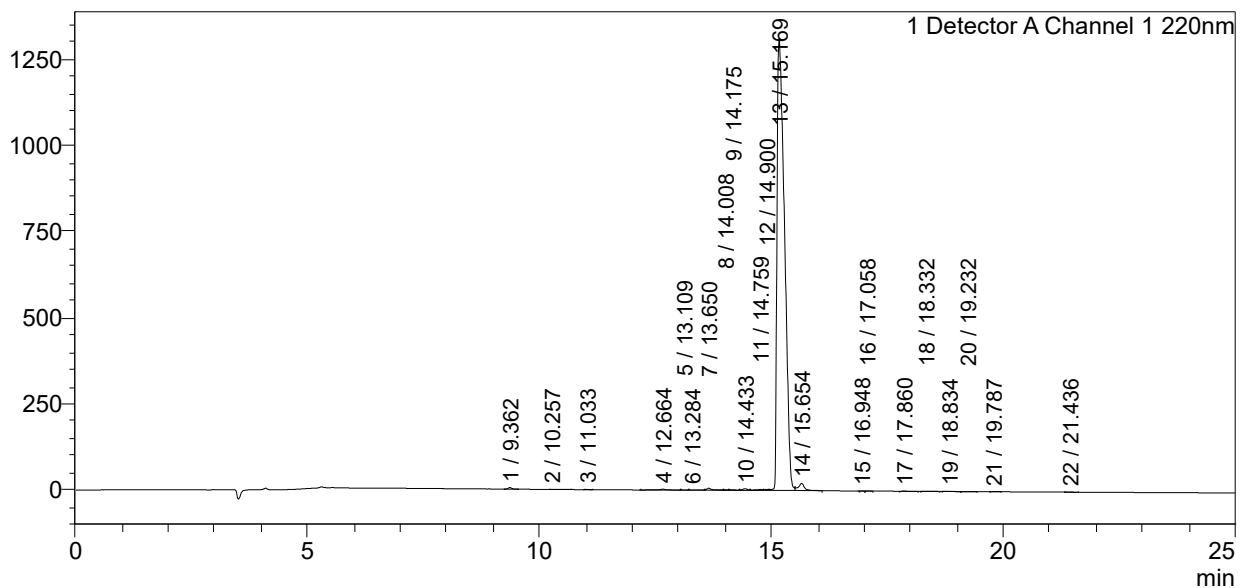

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.362	24772	4660	0.164
2	10.257	1727	179	0.011
3	11.033	1619	294	0.011
4	12.664	30639	2469	0.203
5	13.109	2016	354	0.013
6	13.284	5388	396	0.036
7	13.650	56834	5762	0.376
8	14.008	8763	1315	0.058
9	14.175	13506	1287	0.089
10	14.433	39004	4957	0.258
11	14.759	30737	2853	0.203
12	14.900	19774	2917	0.131
13	15.169	14661337	1313621	97.058
14	15.654	190183	20950	1.259
15	16.948	1509	230	0.010

Peak#	Ret. Time	Area	Height	Area%
16	17.058	2104	314	0.014
17	17.860	3886	458	0.026
18	18.332	2088	178	0.014
19	18.834	3238	265	0.021
20	19.232	3165	294	0.021
21	19.787	1216	134	0.008
22	21.436	2229	290	0.015
Total		15105738	1364175	100.000