

Sample Name:C-Peptide (3-33), human  
 Cat No. : RP11116  
 Lot No.:E5962620C  
 Time Processed: 1:07:40 PM  
 Month-Day-Year Processed :03/27/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm  
 <<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
31.00	Pumps	Pump A B.Conc	5
31.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment:ZJ19010325

<Chromatogram>

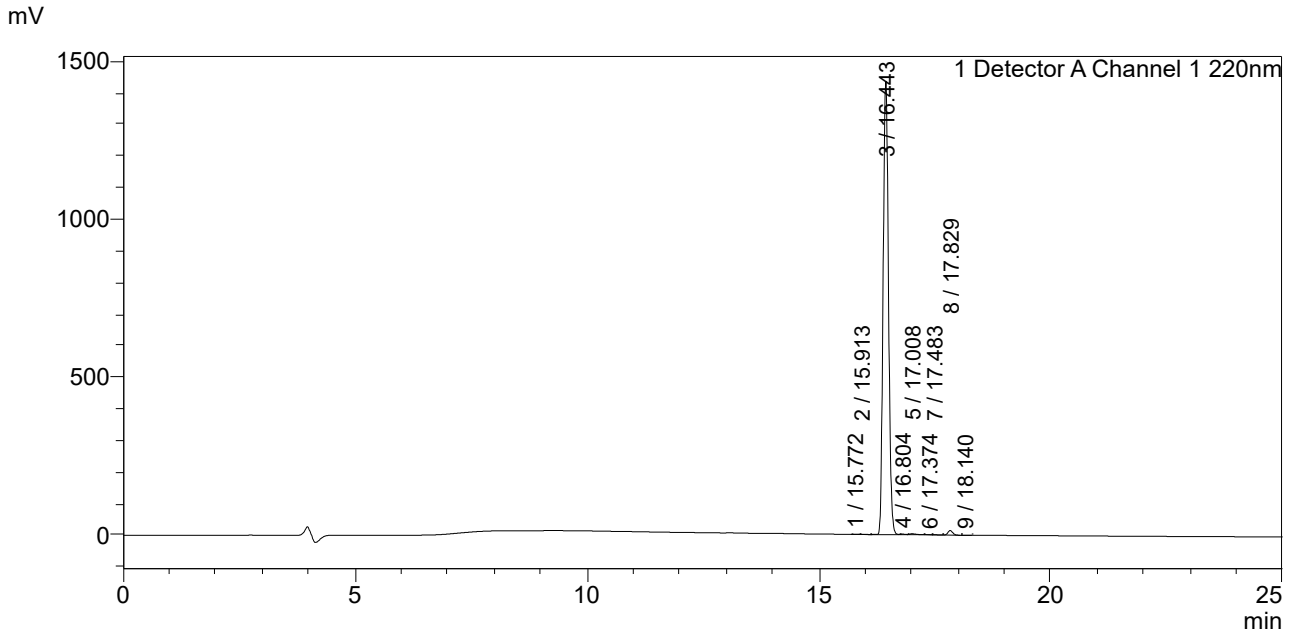

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.772	1770	236	0.015
2	15.913	2215	331	0.019
3	16.443	11498329	1433635	98.609
4	16.804	13883	1778	0.119
5	17.008	31374	3120	0.269
6	17.374	3670	487	0.031
7	17.483	4615	613	0.040
8	17.829	103361	14388	0.886
9	18.140	1322	222	0.011
Total		11660539	1454811	100.000