

Sample Name : OVA G4 peptide  
 Cat. No. : RP20398  
 Lot. No. : E4912220F  
 Time Processed : 4:43:07  
 Month-Day-Year Processed : 07/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

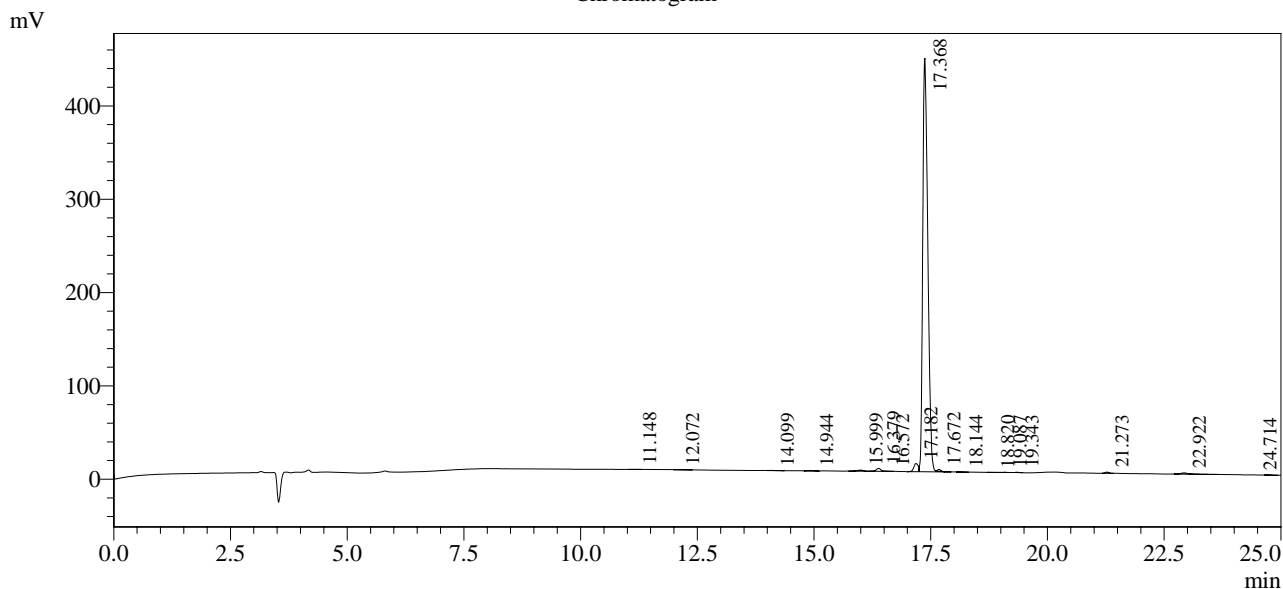

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.148	2195	273	0.063
2	12.072	1791	201	0.051
3	14.099	2467	294	0.071
4	14.944	1978	264	0.057
5	15.999	13187	1177	0.378
6	16.379	24060	3220	0.689
7	16.572	2042	315	0.058
8	17.182	58168	8747	1.666
9	17.368	3343591	443097	95.748
10	17.672	9325	1880	0.267
11	18.144	1568	210	0.045
12	18.820	1073	123	0.031
13	19.087	1577	295	0.045
14	19.343	1968	400	0.056
15	21.273	7358	1290	0.211
16	22.922	18647	1385	0.534
17	24.714	1063	152	0.030
Total		3492058	463323	100.000