

Sample Name : Bradykinin
 Cat. No. : RP11129
 Lot. No. : E6778019J
 Time Processed : 7:38:00
 Month-Day-Year Processed : 11/01/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

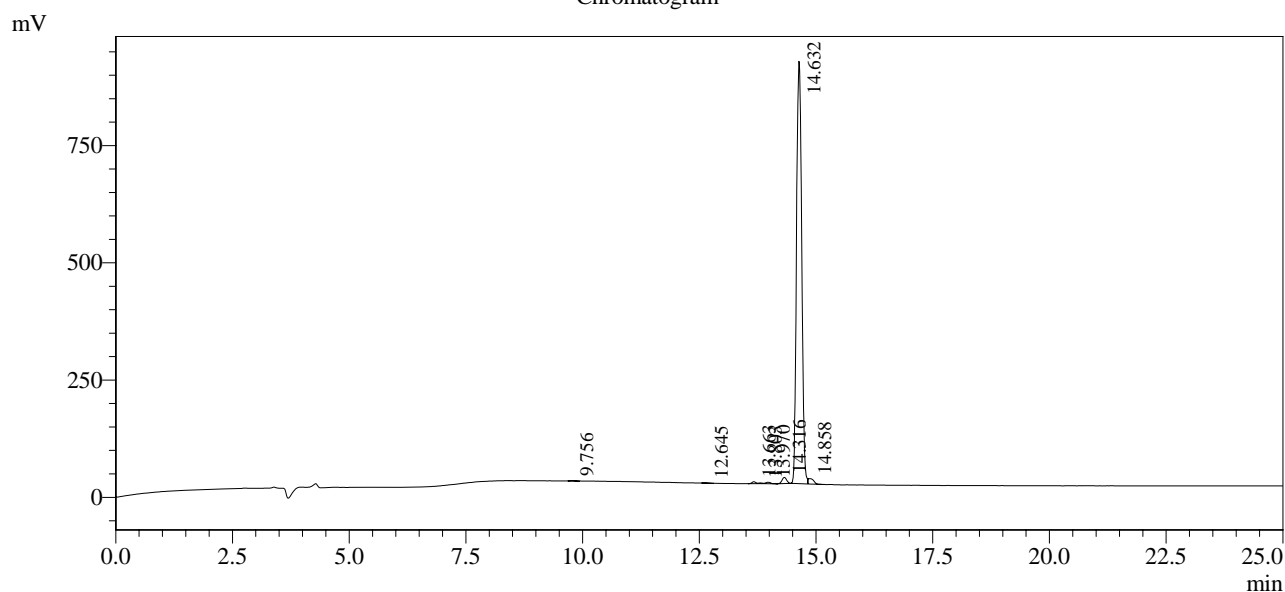

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.756	2902	364	0.040
2	12.645	3703	585	0.051
3	13.663	25419	4155	0.351
4	13.803	9607	1678	0.133
5	13.970	23046	3393	0.318
6	14.316	89778	13156	1.239
7	14.632	7001664	900454	96.619
8	14.858	90572	11313	1.250
Total		7246690	935097	100.000