

Sample Name :VIP, human, ovine, porcine, rat
 Cat No: RP10085
 Lot No : E1513721H
 Time Processed :3:15:38
 Month-Day-Year Processed :08/28/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

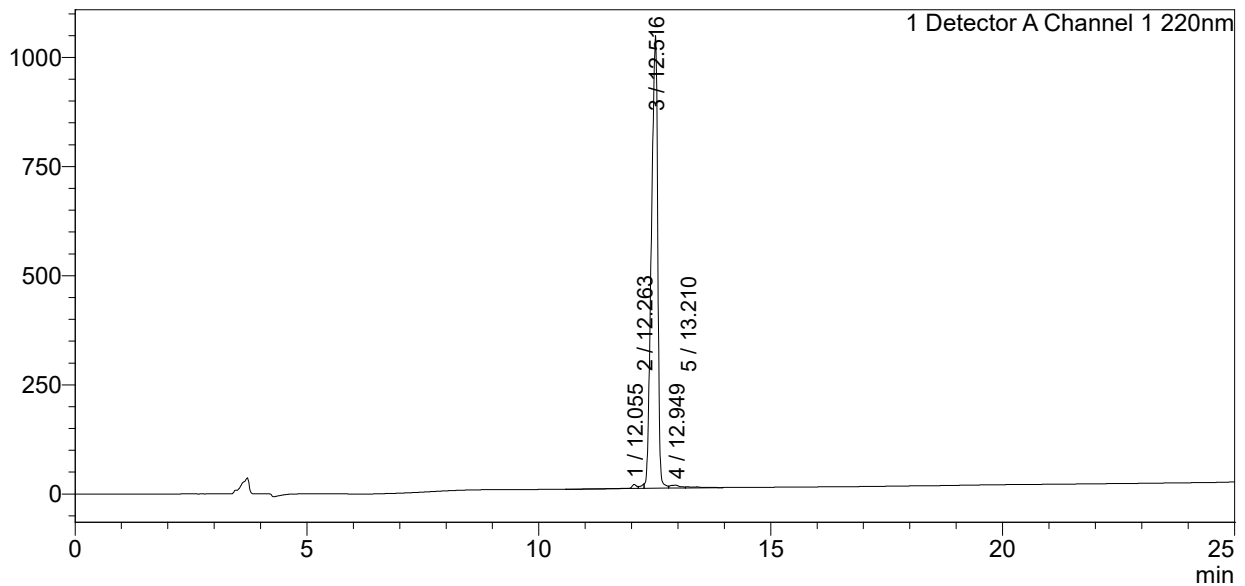

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.055	66391	9280	0.660
2	12.263	47831	9526	0.475
3	12.516	9797494	1037031	97.341
4	12.949	100393	6876	0.997
5	13.210	53062	2518	0.527
Total		10065171	1065230	100.000