

Sample Name :Tuftsin
 Cat No. : RP10624
 Lot No. : E1282620J
 Time Processed : 22:50:54
 Month-Day-Year Processed : 10/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	0
5.00	Pumps	Pump B Conc.	0
20.00	Pumps	Pump B Conc.	30
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
31.00	Pumps	Pump B Conc.	95
31.01	Pumps	Pump B Conc.	0
40.00	Pumps	Pump B Conc.	0
40.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment:GK12010012

<Chromatogram>

mV

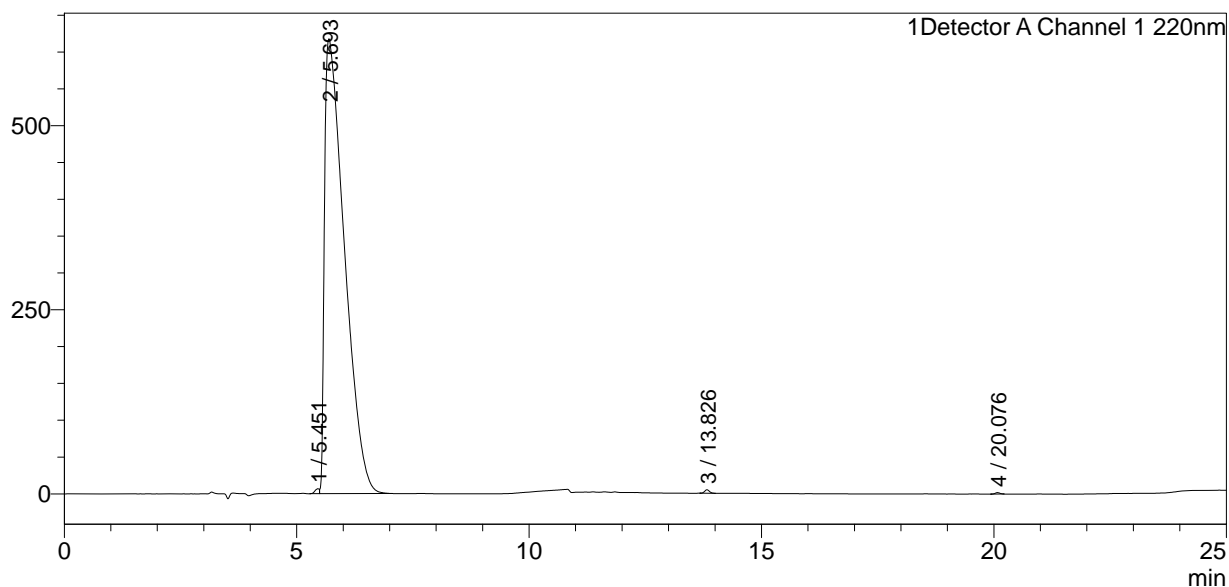

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.451	43593	6674	0.236
2	5.693	18373675	617605	99.510
3	13.826	33625	4662	0.182
4	20.076	13233	1960	0.072
Total		18464126	630901	100.000