


# Mass Spectrum

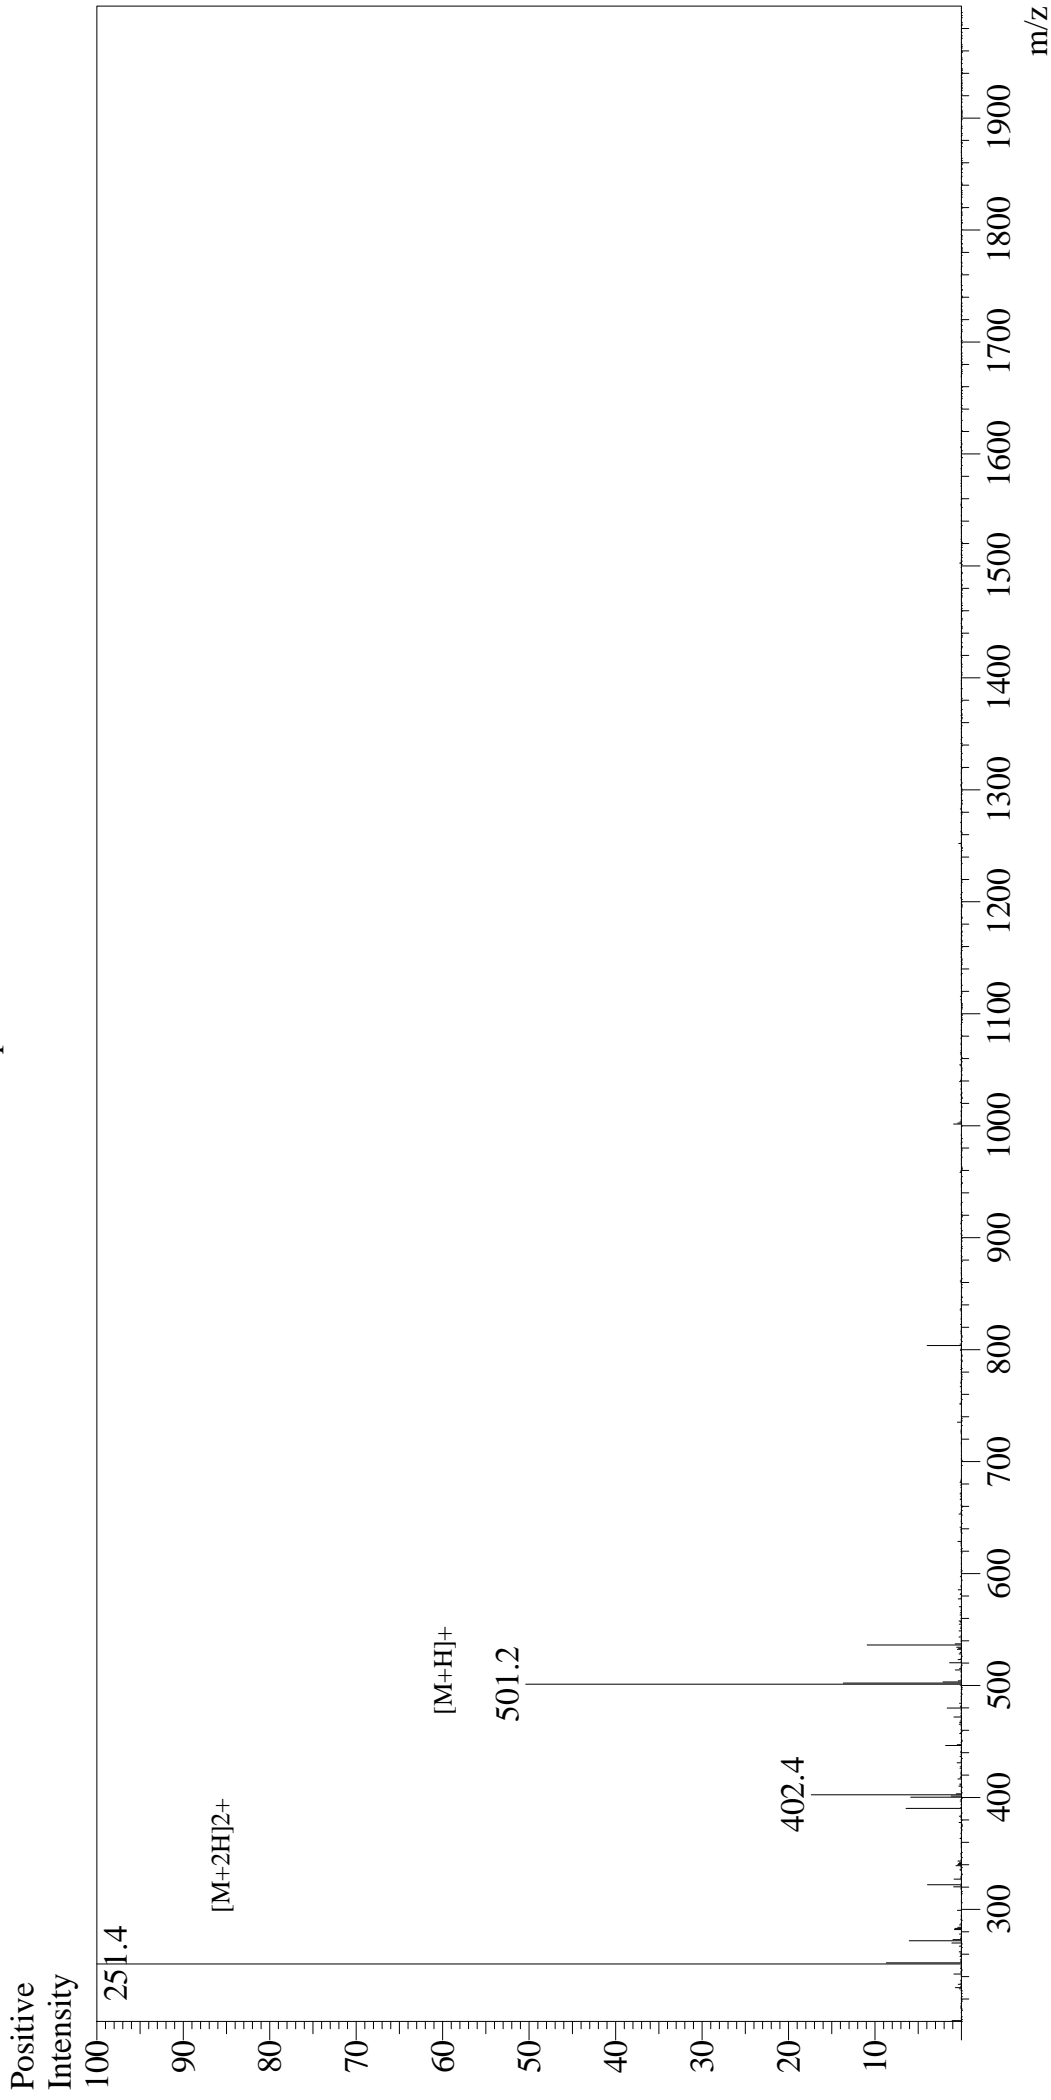

## Sample Information

Month-Day Processed : 10/27/20  
Time Processed : 21:33:49  
Injection Volume : 0.3  
Sample Name : Tuftsin  
Cat No. : RP10624  
Lot No. : E1282620J  
Theoretical MW : 500.60  
Observed MW : 500.8

Interface : ESI  
Nebulizing Gas Flow : 1.5L/min  
CDL Temp : 250  
Block Temp : 200

Equipment : GK11010007  
Interface Bias : +4.5kV  
Drying Gas Flow : 5 L/min  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH