

Sample Name :  $\beta$ -Amyloid (1-40)  
 Cat No. : RP10004  
 Lot No. : E8130721B  
 Time Processed :16:43:30  
 Month-Day-Year Processed :04/04/2021


Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

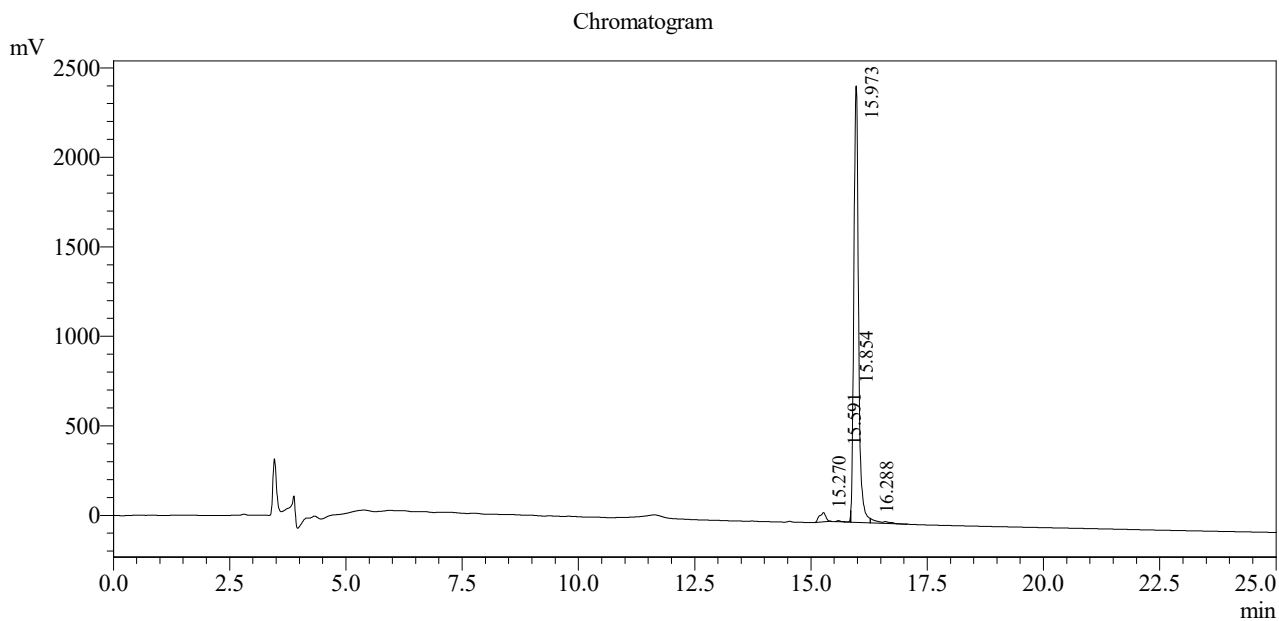

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.270	490145	51104	2.716
2	15.591	26957	5723	0.149
3	15.854	66634	33293	0.369
4	15.973	17158214	2437960	95.070
5	16.288	305968	23686	1.695
Total		18047918	2551766	100.000