

Sample Name :Crosstide
 Cat. No. : RP20200
 Lot. No. : E4854119I
 Time Processed :8:25:57
 Month-Day-Year Processed : 09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

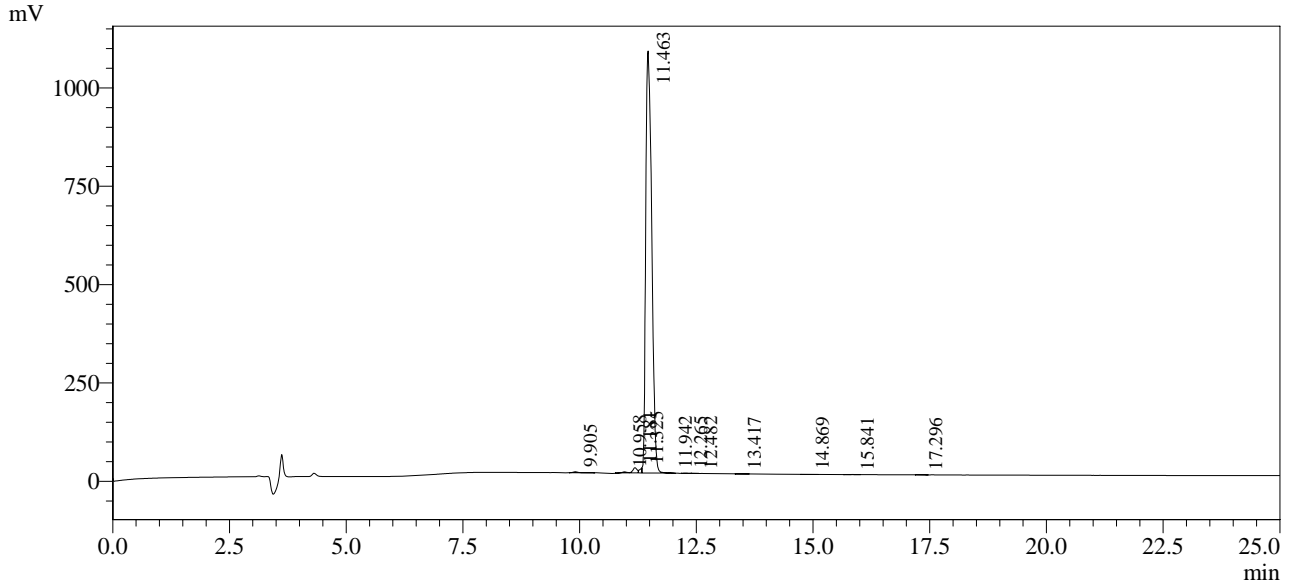

1 Det. A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.905	16864	2370	0.173
2	10.958	18078	2724	0.185
3	11.181	84233	13258	0.863
4	11.325	42127	11520	0.432
5	11.463	9572792	1072671	98.123
6	11.942	1392	343	0.014
7	12.265	3068	580	0.031
8	12.482	1844	368	0.019
9	13.417	5211	853	0.053
10	14.869	6506	765	0.067
11	15.841	2243	267	0.023
12	17.296	1534	182	0.016
Total		9755893	1105901	100.000