

Sample Name :Transdermal Peptide
Cat No. : RP20404
Lot No. :PE6501905
Time Processed : 22:05:21
Month-Day-Year Processed : 06/01/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	0
5.00	Pumps	Pump B Conc.	0
20.00	Pumps	Pump B Conc.	30
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
31.00	Pumps	Pump B Conc.	95
31.01	Pumps	Pump B Conc.	0
40.00	Pumps	Pump B Conc.	0
40.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment:GK12010012

<Chromatogram>

mV

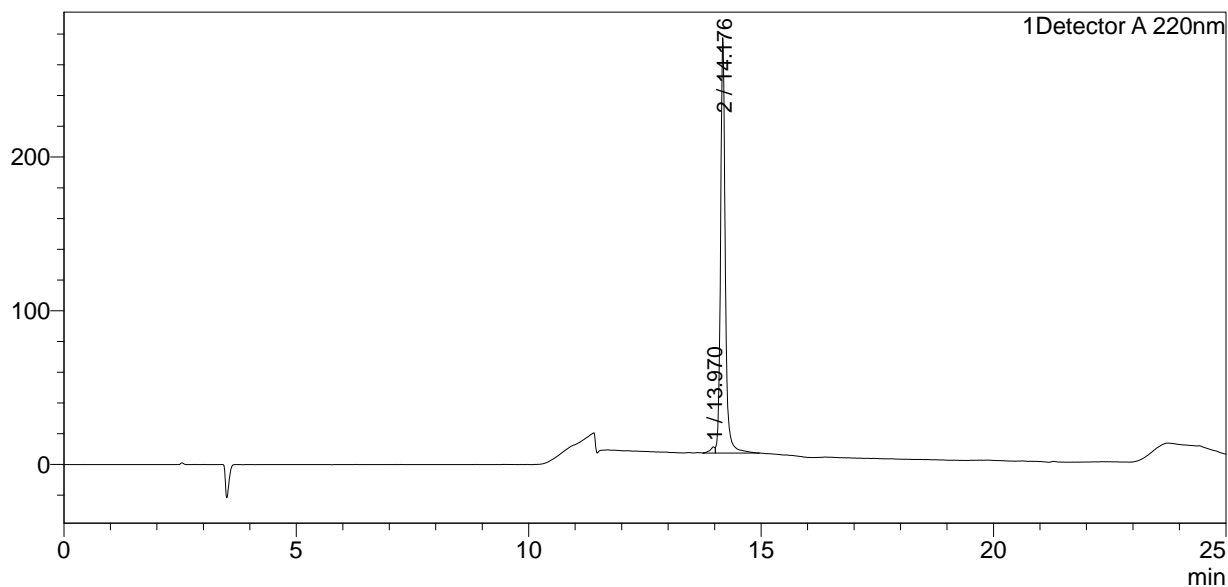

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.970	30028	3985	1.545
2	14.176	1913507	270151	98.455
Total		1943535	274136	100.000