

Sample Name :Influenza NP (147-155)

Cat. No. : RP20260

Lot. No. : E1981621E

Time Processed :22:57:09

Month-Day-Year Processed :05/12/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)

Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)

Total Flow:1 ml/min

Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>


<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: ZJ20010140

### <Chromatogram>

mV

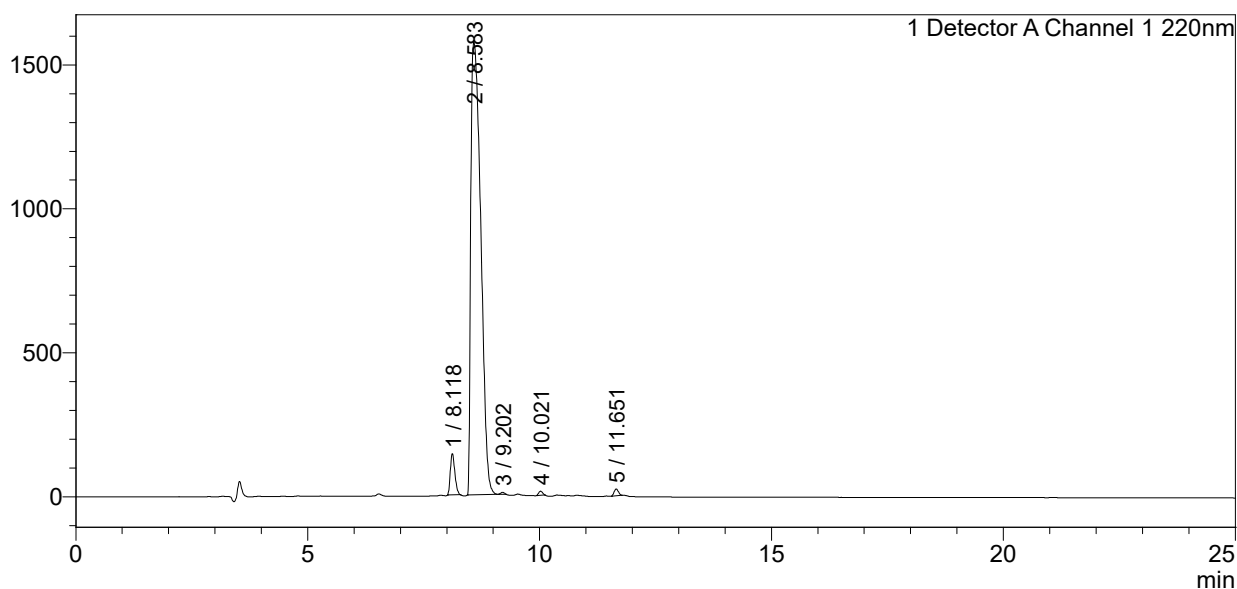

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.118	963483	143212	3.918
2	8.583	23365177	1577938	95.007
3	9.202	34333	6451	0.140
4	10.021	79411	13743	0.323
5	11.651	150709	23533	0.613
Total		24593113	1764876	100.000