

Sample Name : SIYRY  
 Cat. No. :RP20234  
 Lot. No. :PE3541612

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

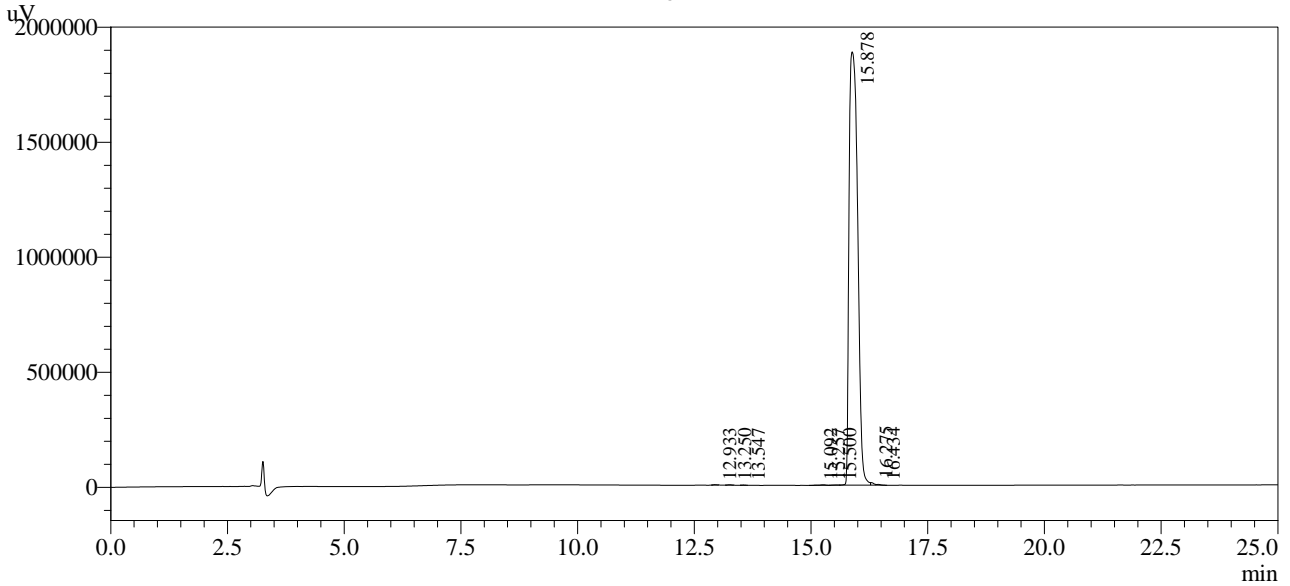

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.933	6565	1372	0.027
2	13.250	9054	1760	0.037
3	13.547	4071	860	0.017
4	15.092	4170	688	0.017
5	15.257	17024	2272	0.070
6	15.500	6662	1163	0.027
7	15.878	24178106	1883510	99.501
8	16.275	52049	11116	0.214
9	16.434	21751	3532	0.090
Total		24299452	1906274	100.000