

Sample Name :SV40 large T antigen NLS
 Cat No.: RP20414
 Lot No.:E4969019I
 Time Processed :14:55:24
 Month-Day-Year Processed :09/27/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	15
25.00	Pumps	Solvent B Conc.	75
25.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	15
40.00	Pumps	Solvent B Conc.	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

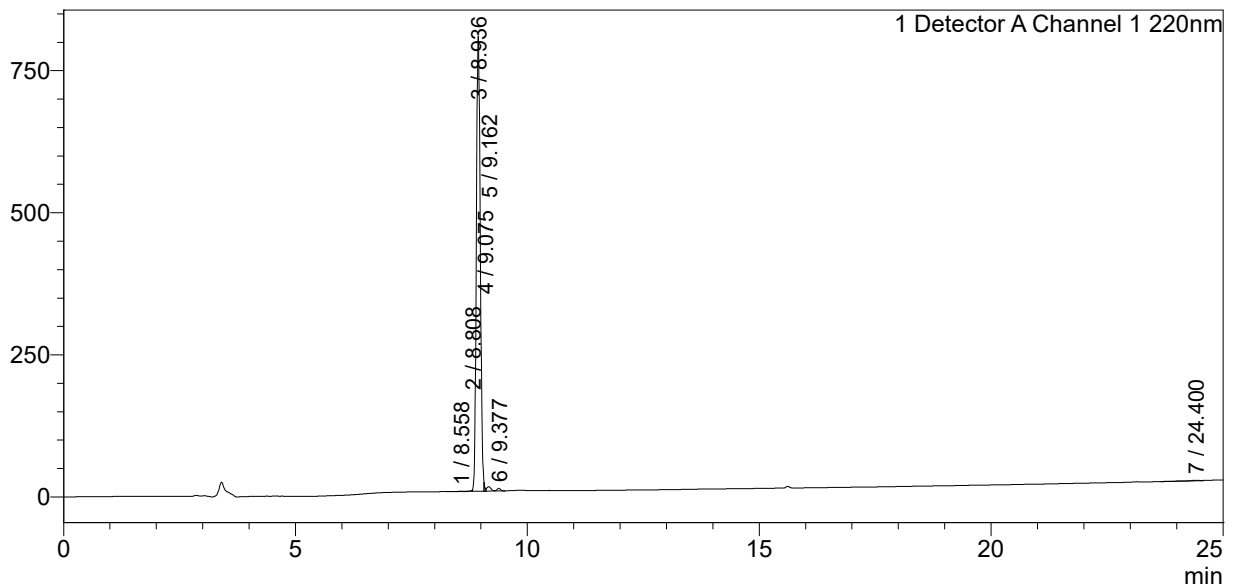

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.558	2421	364	0.050
2	8.808	6297	2057	0.129
3	8.936	4766532	801154	97.885
4	9.075	15408	9902	0.316
5	9.162	46573	7597	0.956
6	9.377	23235	4563	0.477
7	24.400	9056	554	0.186
Total		4869523	826190	100.000