

Sample Name :N-Formyl-Nle-Leu-Phe-Nle-Tyr-Lys
 Cat. No. : RP12959
 Lot. No.: E5567519J
 Time Processed :0:05:45
 Month-Day-Year Processed :10/11/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

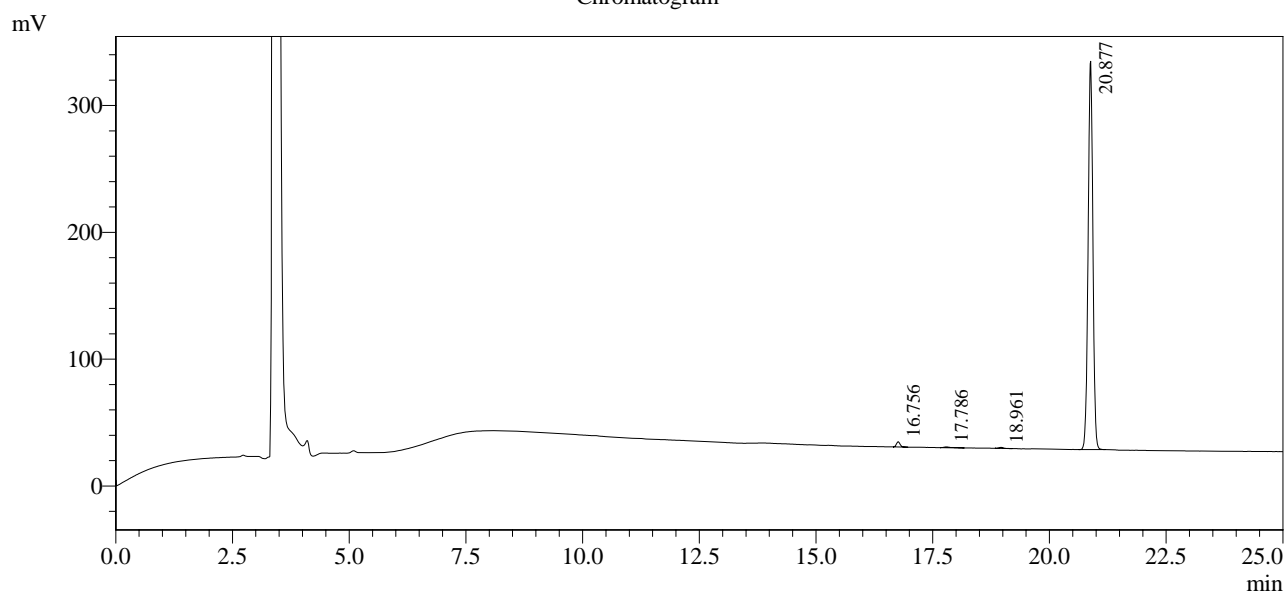

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.756	22015	4073	0.995
2	17.786	6749	614	0.305
3	18.961	5691	827	0.257
4	20.877	2177632	306138	98.442
Total		2212086	311651	100.000