

Sample Name :Gly-Arg-Gly-Asp-Ser
 Cat No. :RP10848
 Lot No. :E6489021B
 Time Processed :7:25:53 PM
 Month-Day-Year Processed :02/15/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	B.Conc	0
5.00	Pumps	B.Conc	0
20.00	Pumps	B.Conc	30
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	0
35.00	Pumps	B.Conc	0
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

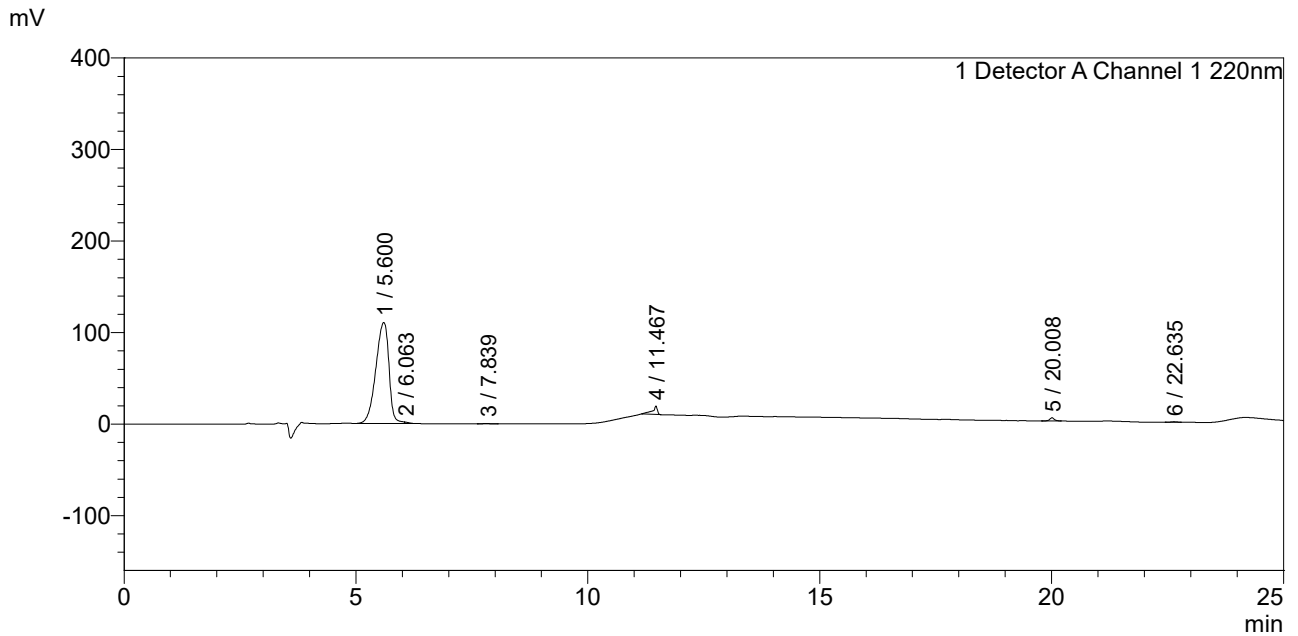

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.600	2166926	110280	95.224
2	6.063	8778	1547	0.386
3	7.839	3347	293	0.147
4	11.467	69728	9300	3.064
5	20.008	23523	3416	1.034
6	22.635	3299	481	0.145
Total		2275601	125317	100.000