

Sample Name: Peptide YY (PYY), human
 Cat No. : RP10355
 Lot No. : E5956120C
 Time Processed: 9:48:50 AM
 Month-Day-Year Processed :03/26/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.10	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm
 Equipment: ZJ19010325

<Chromatogram>

mV

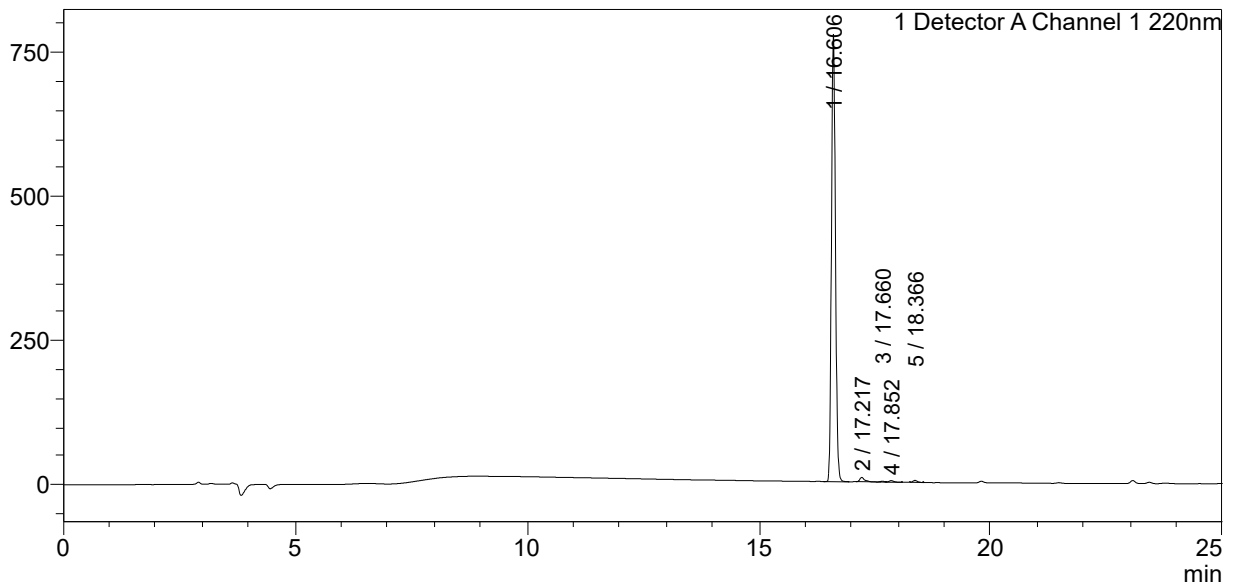

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.606	4623317	776618	97.887
2	17.217	51088	7619	1.082
3	17.660	6864	1344	0.145
4	17.852	18751	2604	0.397
5	18.366	23076	3531	0.489
Total		4723097	791716	100.000