

Sample Name : [Leu5]-Enkephalin
 Cat.No : RP10884
 Lot.No : E6131020J
 Time Processed: 15:33:40
 Year-Month-Day: 2020/10/30

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min

<<Detector A>>
 Wavelength Ch1 : 220 nm

<<LC Time Program>>


Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010015

<Chromatogram>

mV

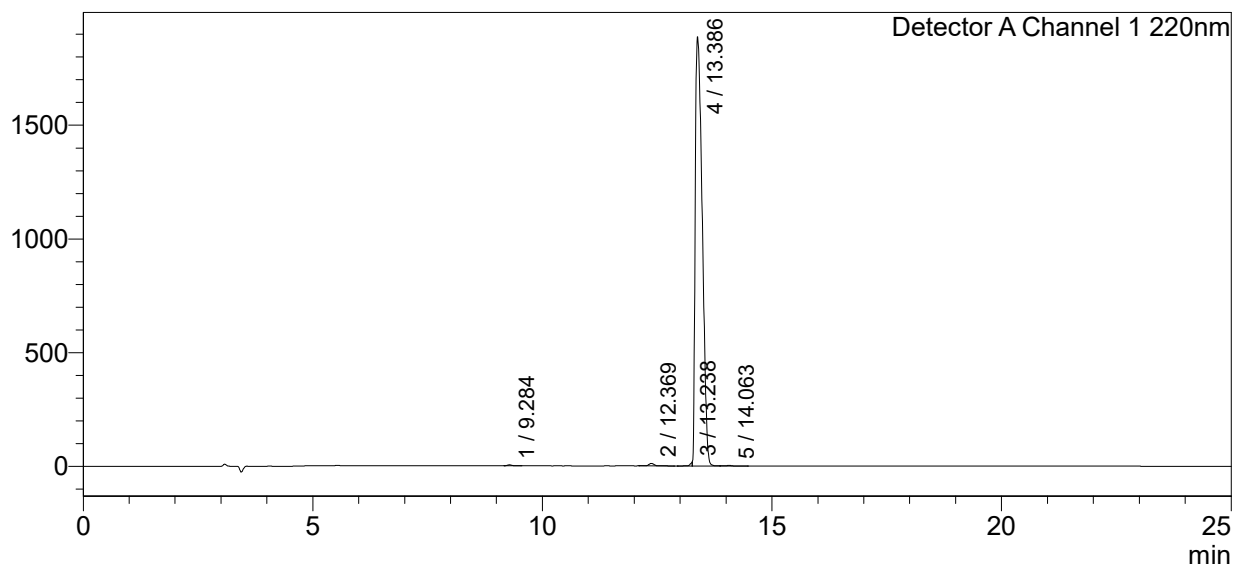

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.284	29663	4467	0.147
2	12.369	88077	10577	0.437
3	13.238	52129	8011	0.259
4	13.386	19942946	1868049	99.033
5	14.063	24959	2399	0.124
Total		20137774	1893504	100.000