

Sample Name :Angiotensin II, human
 Cat. No. : RP11257
 Lot. No. : E2516620J
 Time Processed :22:20:03

Month-Day-Year Processed :10/17/2020
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010324

<Chromatogram>

mV

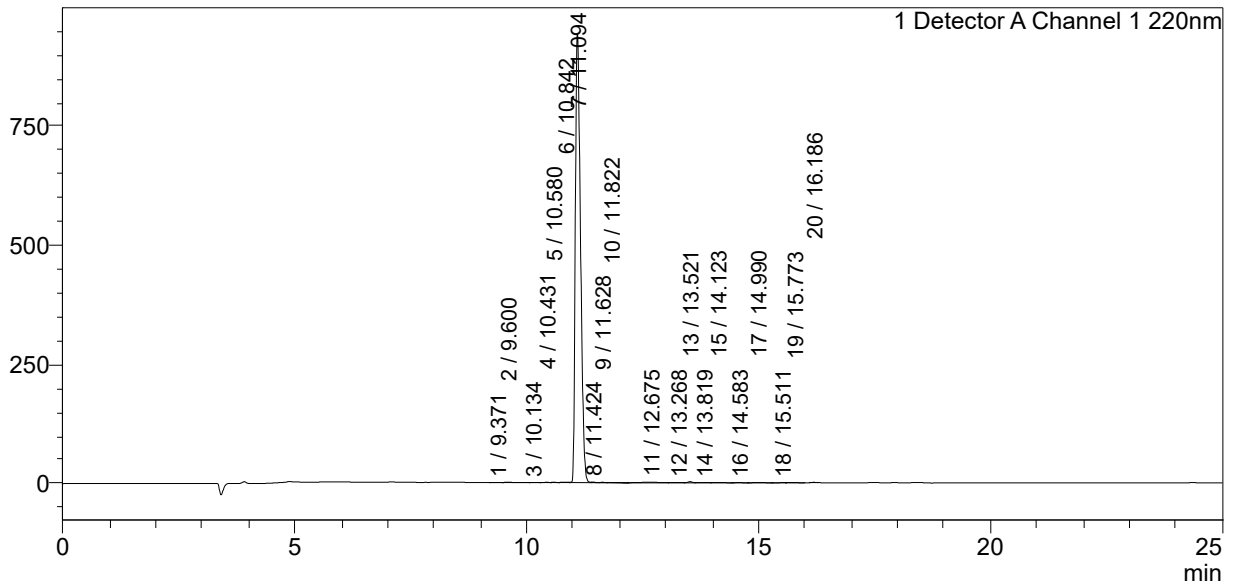

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.371	4074	366	0.054
2	9.600	12104	614	0.161
3	10.134	1095	166	0.015
4	10.431	5111	598	0.068
5	10.580	6058	754	0.081
6	10.842	13396	1102	0.178
7	11.094	7342377	942486	97.656
8	11.424	1049	242	0.014
9	11.628	5110	604	0.068
10	11.822	8053	596	0.107
11	12.675	36658	1080	0.488
12	13.268	11525	814	0.153
13	13.521	16853	2375	0.224
14	13.819	9836	545	0.131
15	14.123	11358	646	0.151
16	14.583	5042	448	0.067

Peak#	Ret. Time	Area	Height	Area%
17	14.990	13161	825	0.175
18	15.511	5383	366	0.072
19	15.773	8238	546	0.110
20	16.186	2136	431	0.028
Total		7518618	955602	100.000