

Sample Name : CLIP (86-100)
 Cat No. : RP20279
 Lot No. : E3757021B
 Time Processed: 6:34:42
 Year-Month-Day: 2021/2/3

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min

<<Detector A>>

Wavelength Ch1 : 220 nm

<<LC Time Program>>

Time	Module	Command	Value	Comment
0.01	Pumps	Solvent B Conc.	5	
25.00	Pumps	Solvent B Conc.	65	
25.01	Pumps	Solvent B Conc.	95	
27.00	Pumps	Solvent B Conc.	95	
27.01	Pumps	Solvent B Conc.	5	
33.00	Pumps	Solvent B Conc.	5	
33.01	Controller	Stop		

<<Column Performance>>


<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment:ZJ19010015

<Chromatogram>

mV

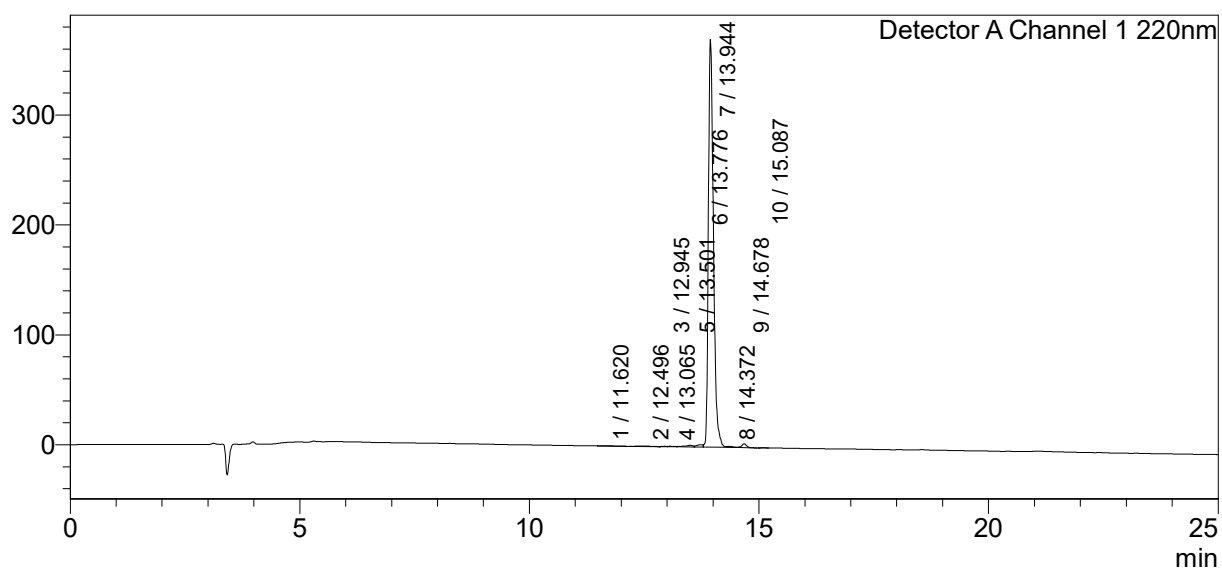

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.620	5698	234	0.193
2	12.496	6813	341	0.230
3	12.945	3349	443	0.113
4	13.065	4376	501	0.148
5	13.501	19844	1593	0.671
6	13.776	19483	2127	0.659
7	13.944	2866409	370837	96.976
8	14.372	2890	524	0.098
9	14.678	25229	3494	0.854
10	15.087	1694	253	0.057
Total		2955784	380347	100.000