

Sample Name :Neurokinin A (4-10)
 Cat No. :RP10516
 Lot No. :E6812019J
 Time Processed :10:19:42 AM
 Month-Day-Year Processed :10/16/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
30.01	Pumps	Solvent B Conc.	95
31.00	Pumps	Solvent B Conc.	95
31.01	Pumps	Solvent B Conc.	5
40.00	Pumps	Solvent B Conc.	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

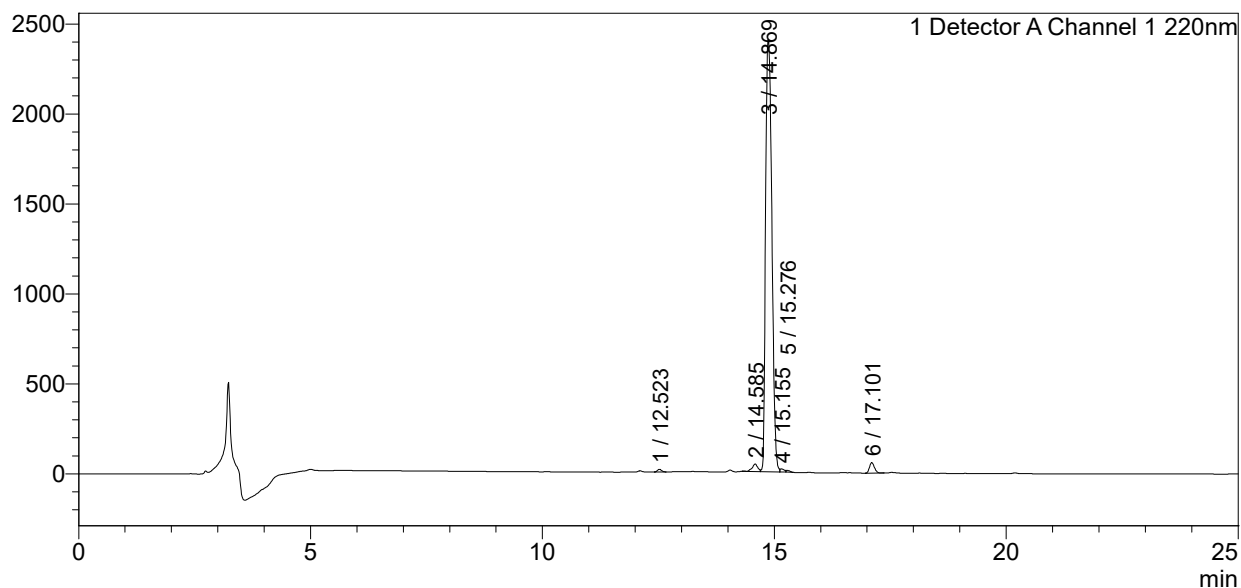

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.523	87951	14539	0.374
2	14.585	348435	42057	1.480
3	14.869	22534160	2403487	95.699
4	15.155	98520	16716	0.418
5	15.276	45542	9045	0.193
6	17.101	432192	58571	1.835
Total		23546799	2544416	100.000