

Sample Name :Substance P, Free Acid
 Cat No. :RP10185
 Lot No. :E4689919I
 Time Processed :4:28:35
 Month-Day-Year Processed :09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

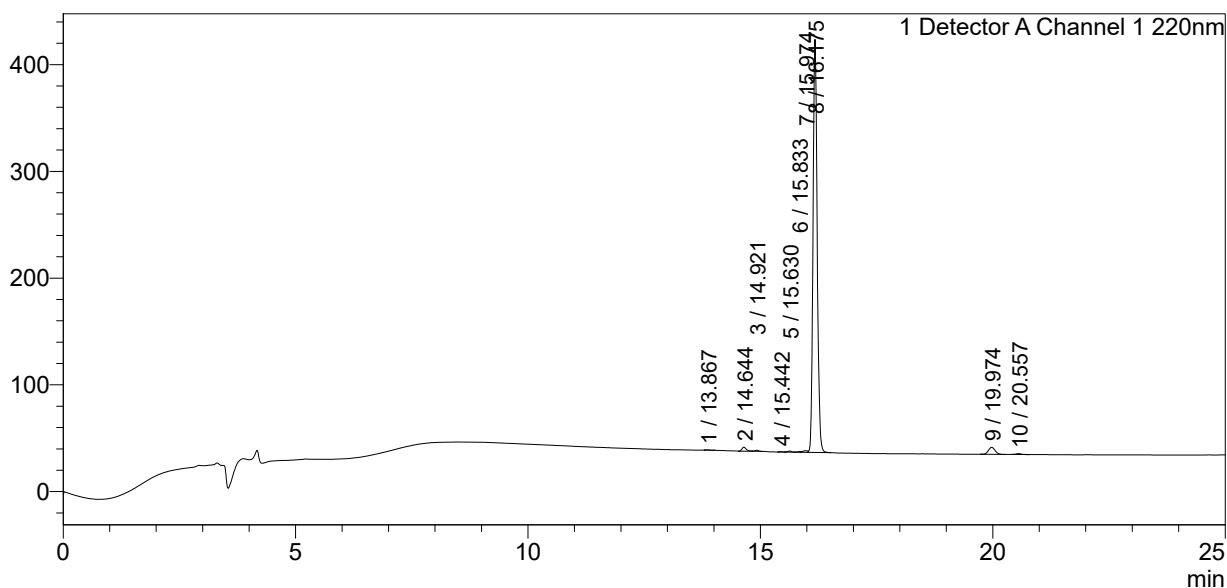

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.867	1487	292	0.059
2	14.644	24544	3775	0.968
3	14.921	5355	984	0.211
4	15.442	2079	329	0.082
5	15.630	6494	1005	0.256
6	15.833	3051	655	0.120
7	15.974	11240	1549	0.443
8	16.175	2410603	386926	95.031
9	19.974	65961	6573	2.600
10	20.557	5846	757	0.230
Total		2536660	402844	100.000