

Sample Name :Hexa-His
 Cat No. :RP11737
 Lot No. :E1778419K
 Time Processed :8:06:24
 Month-Day-Year Processed :11/10/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

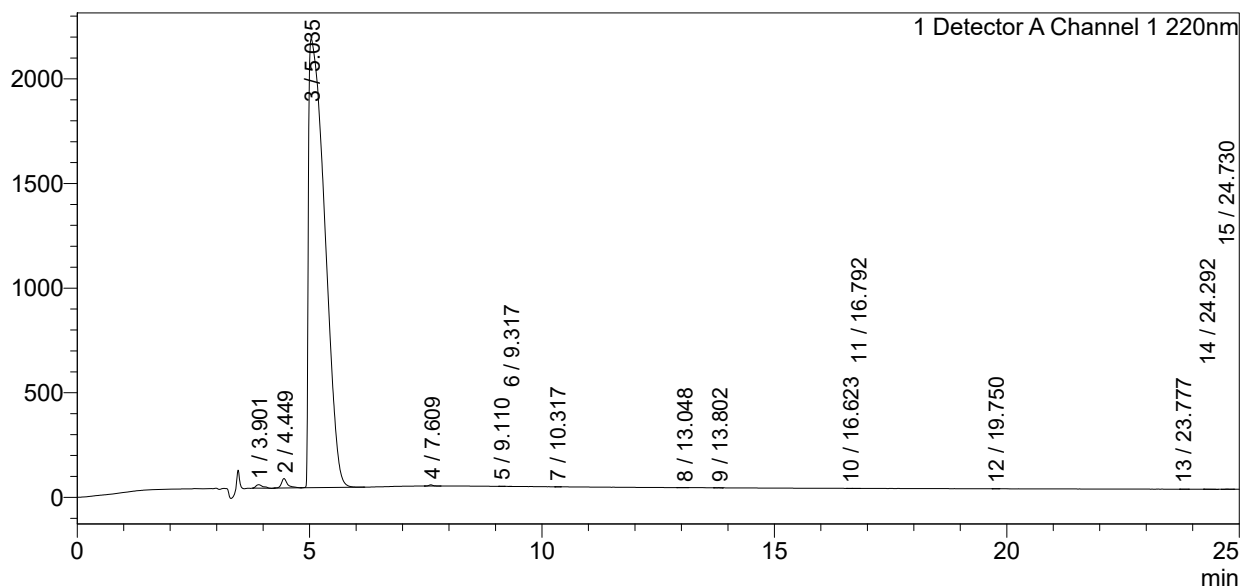

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	3.901	172911	16609	0.328
2	4.449	407552	45112	0.774
3	5.035	52015064	2146861	98.785
4	7.609	33750	5717	0.064
5	9.110	1051	342	0.002
6	9.317	1515	270	0.003
7	10.317	1099	264	0.002
8	13.048	2423	279	0.005
9	13.802	4139	787	0.008
10	16.623	1178	269	0.002
11	16.792	1055	167	0.002
12	19.750	1483	409	0.003
13	23.777	1170	259	0.002
14	24.292	2551	202	0.005
15	24.730	7865	1038	0.015

Peak#	Ret. Time	Area	Height	Area%
Total		52654805	2218585	100.000