


Mass Spectrum

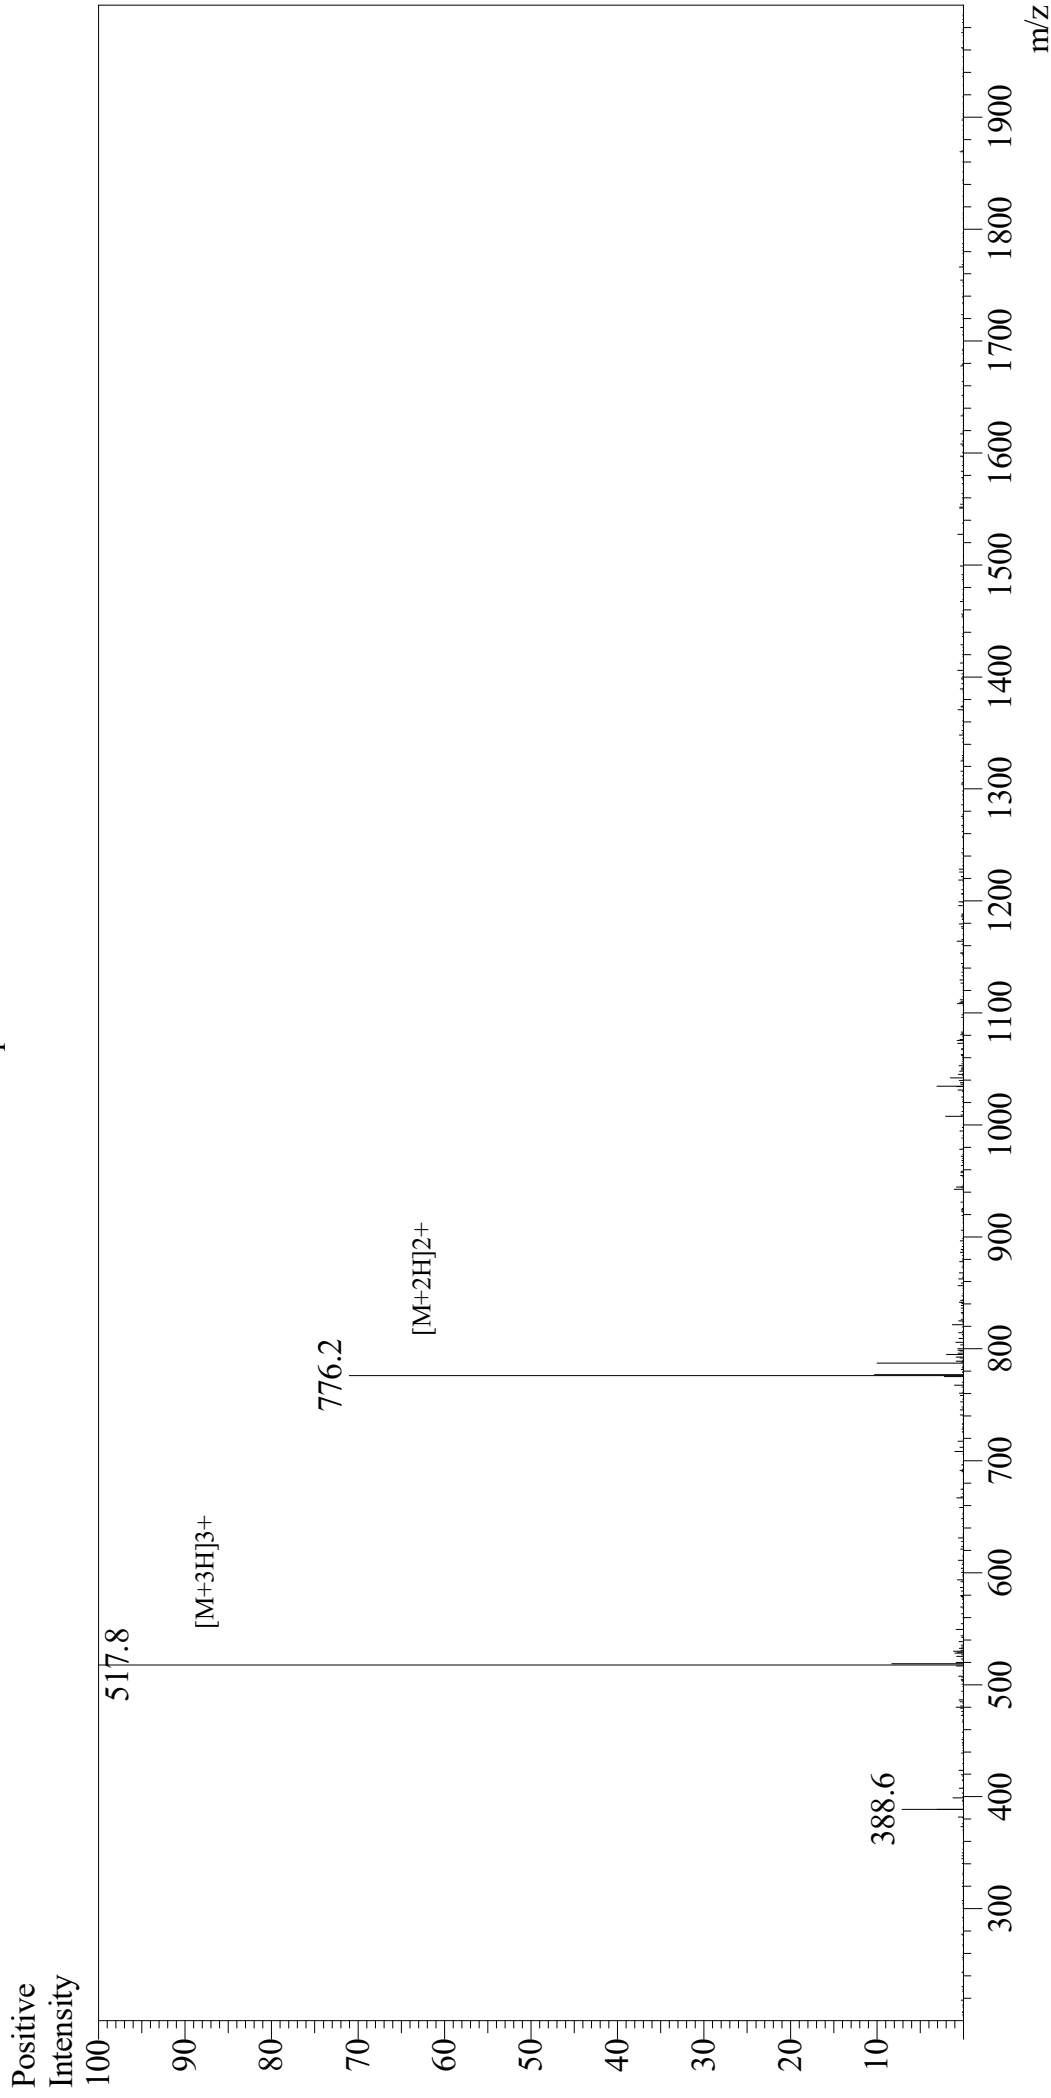

Sample Information

User : Gary
Month-Day Processed : 04/01/20
Time Processed : 11:19:02 AM
Injection Volume : 0.3
Sample Name : 43Gap 26, Connexin Mimetic
Cat No. : RP20274
Lot No. : E6430120C
Theoretical MW : 1550.79
Observed MW : 1550.4

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200