


Mass Spectrum

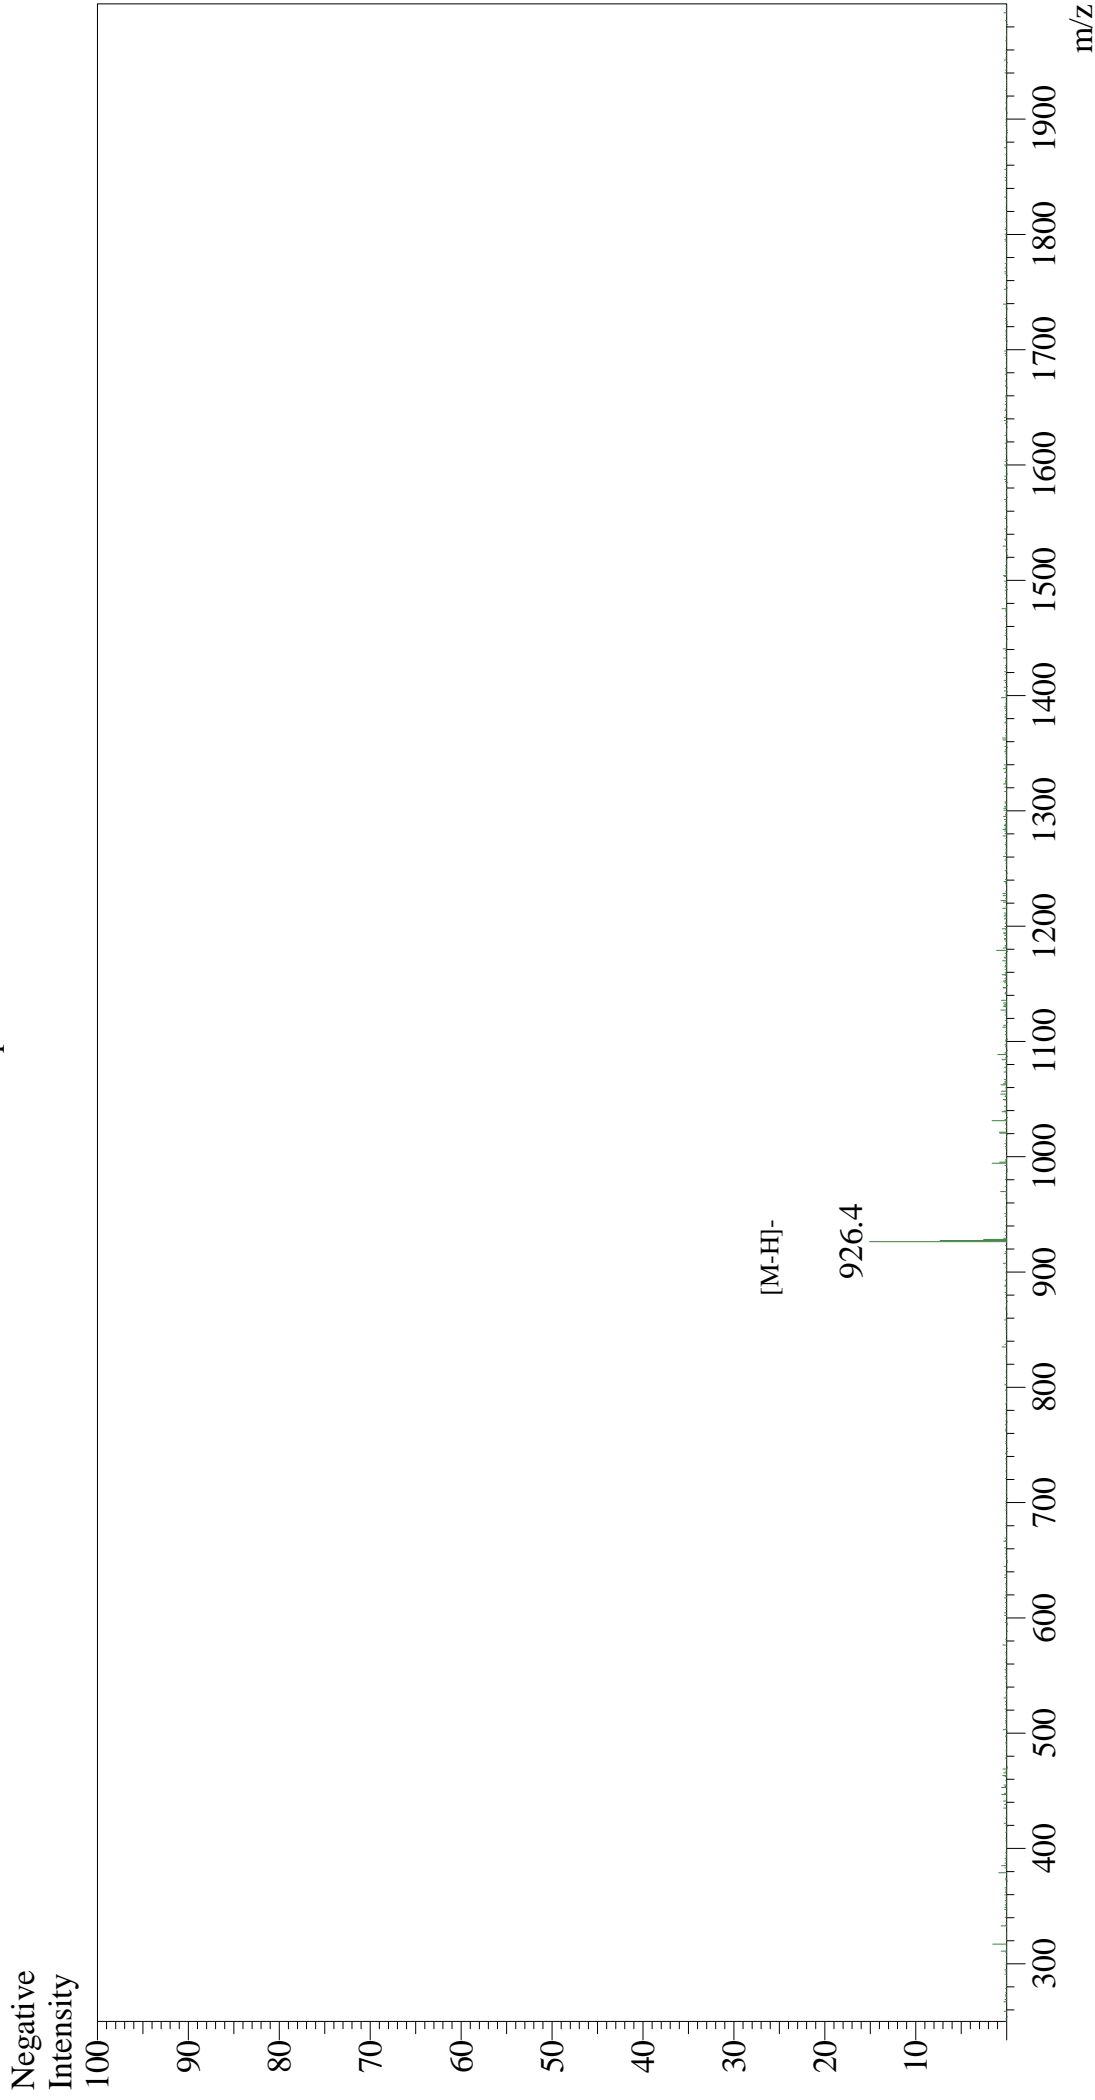

Sample Information

User : Gary
Month-Day Processed : 01/22/20
Time Processed : 17:49:32
Injection Volume : 0.3
Sample Name : Bacterial Sortase Substrate III, Abz/DNP
Cat No. : RP20431
Lot No. : E6205820A
Theoretical MW : 928.00
Observed MW : 927.4

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : -3.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50%H2O/50%MeOH