

Sample Name : Corticotropin Releasing Factor, human, rat
Cat. No. : RP10982
Lot. No. :PE3451612

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
Total Flow:1 ml/min
Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

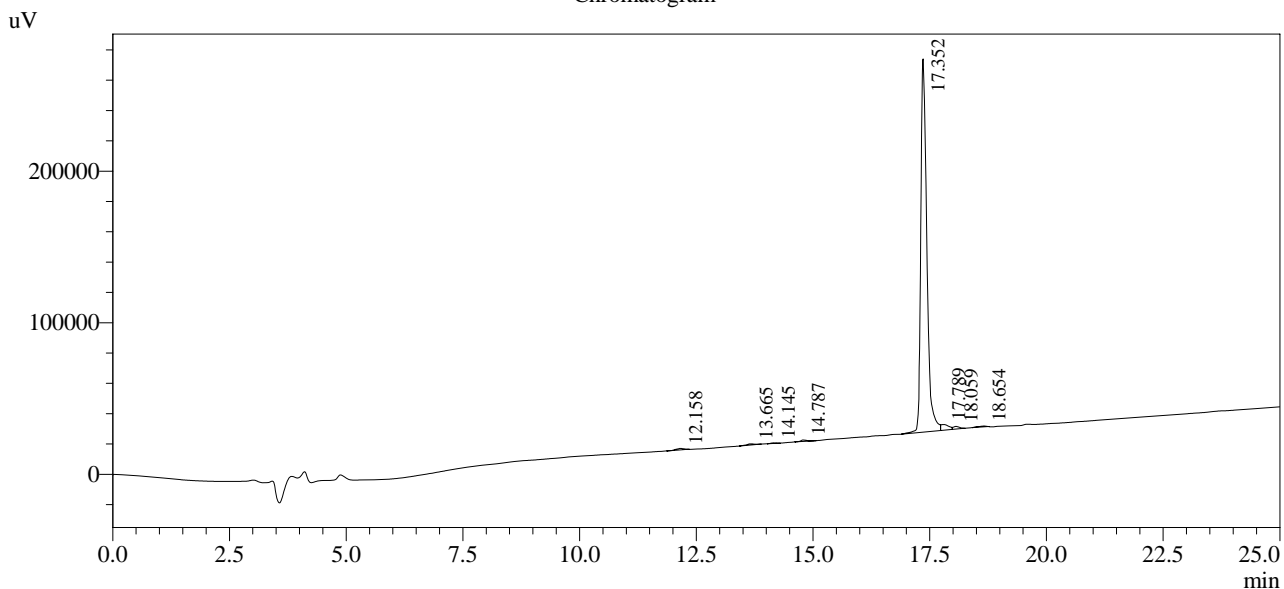

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.158	11601	991	0.501
2	13.665	8907	768	0.385
3	14.145	3066	384	0.132
4	14.787	7849	961	0.339
5	17.352	2215877	246332	95.765
6	17.789	43145	3790	1.865
7	18.059	16171	1797	0.699
8	18.654	7245	559	0.313
Total		2313861	255583	100.000