

Sample Name : [Met⁵]-Enkephalin
 Cat. No. : RP10886
 Lot. No. : PE9371703

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

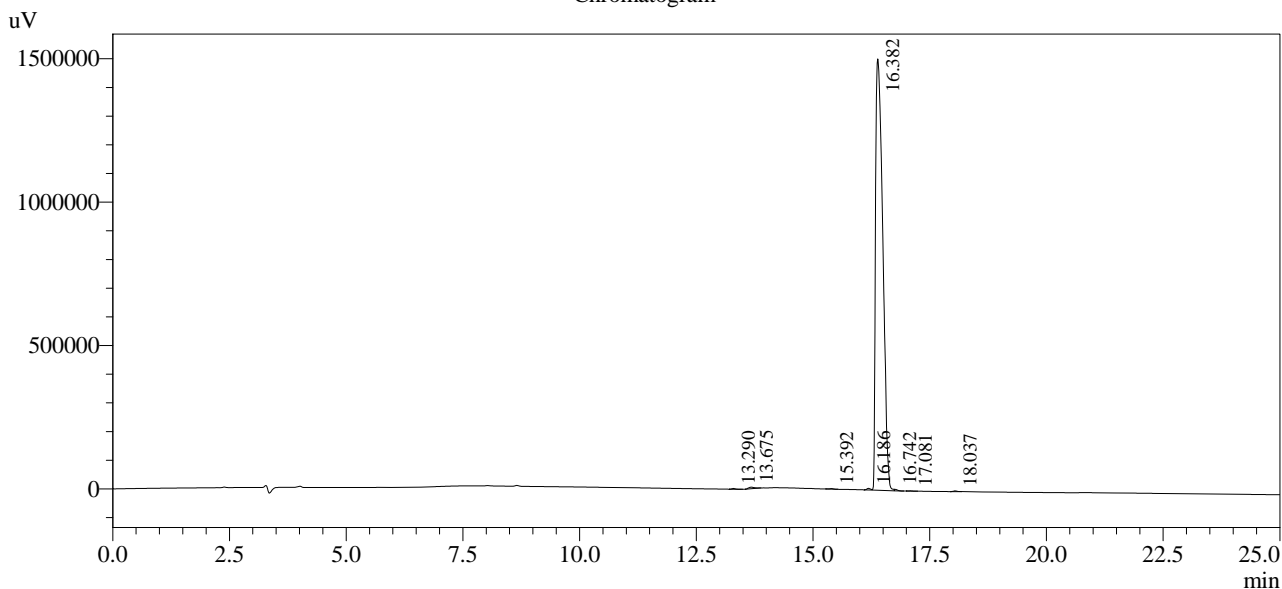

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.290	12941	2481	0.079
2	13.675	50712	5539	0.309
3	15.392	10163	1790	0.062
4	16.186	31200	5657	0.190
5	16.382	16261407	1504553	99.116
6	16.742	21613	5083	0.132
7	17.081	4226	768	0.026
8	18.037	14225	2594	0.087
Total		16406487	1528464	100.000