

Sample Name : Gastrin-1, human
 Cat. No. : RP12740-0.5
 Lot. No. : PE6151709

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Chromatogram

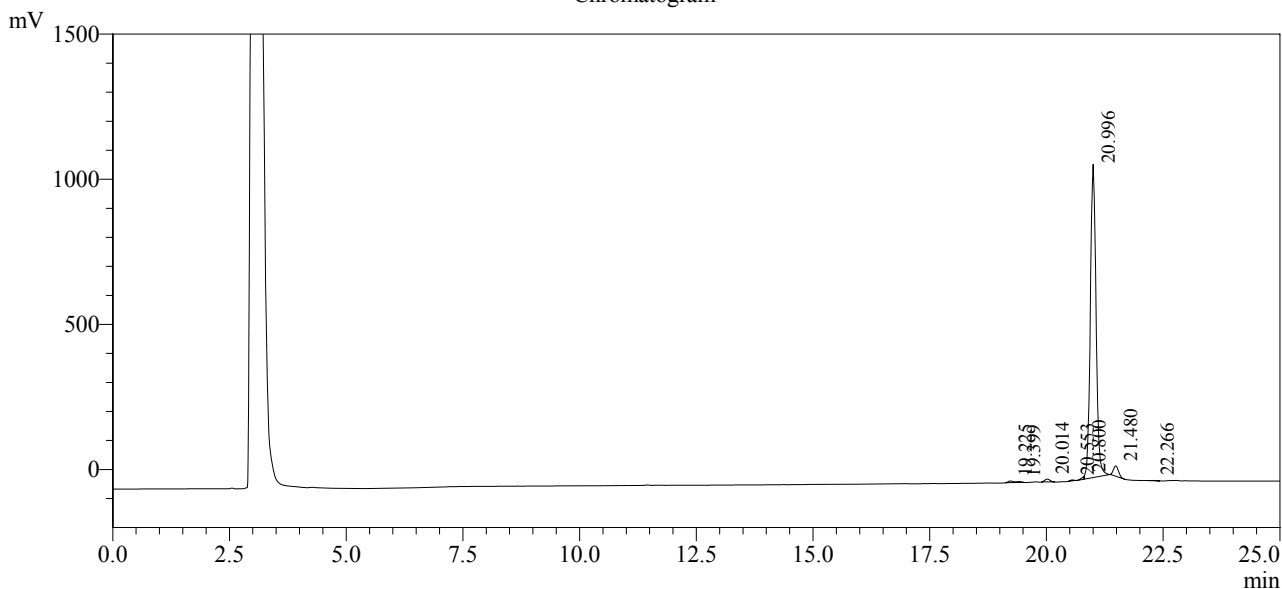

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	19.225	41775	5619	0.434
2	19.399	18206	2596	0.189
3	20.014	76155	9808	0.791
4	20.553	16932	3074	0.176
5	20.800	39868	9226	0.414
6	20.996	9164910	1078795	95.139
7	21.480	265728	35430	2.758
8	22.266	9651	1423	0.100
Total		9633224	1145970	100.000