

Sample Name :Cardiotoxin Analog (CTX) IV (6-12)
 Cat No. :RP17303
 Lot No. :E4906319I
 Time Processed :9:49:48 AM
 Month-Day-Year Processed :09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

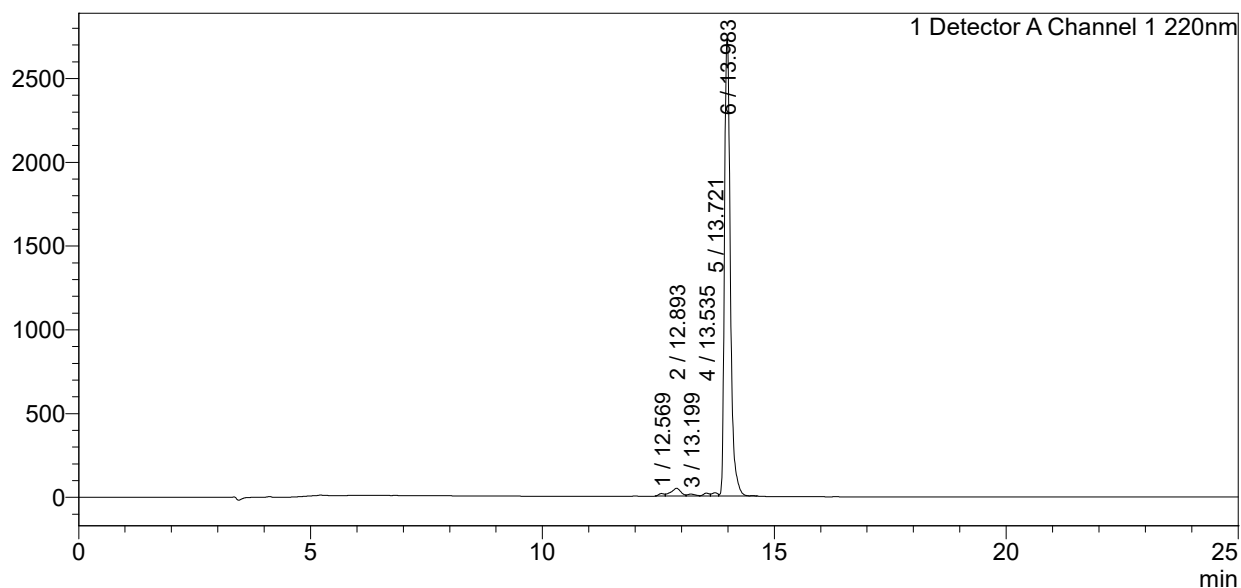

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	12.569	130420	14936	0.513
2	12.893	679919	46947	2.675
3	13.199	132704	11289	0.522
4	13.535	158130	17189	0.622
5	13.721	165934	20018	0.653
6	13.983	24147505	2727693	95.014
Total		25414611	2838072	100.000