


Mass Spectrum

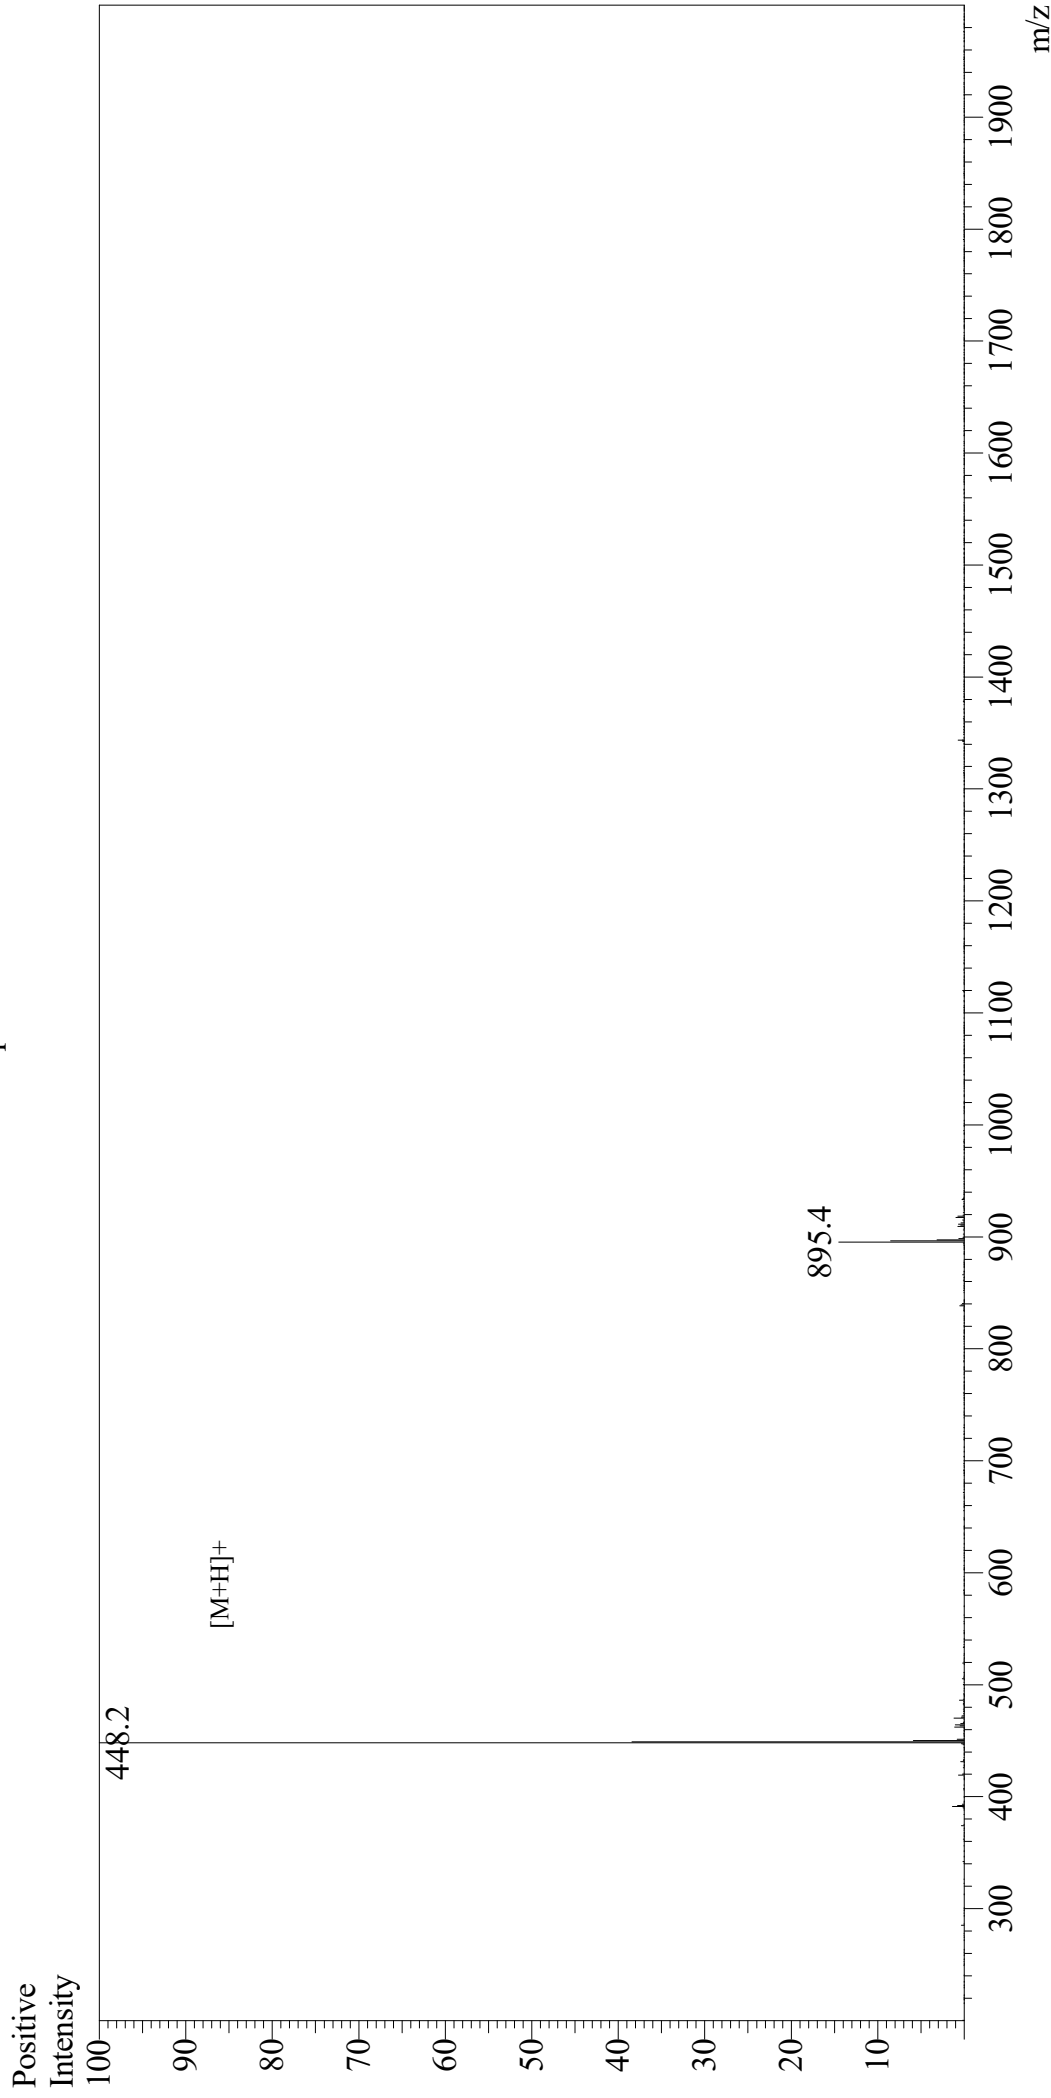

Sample Information

User : Gary
Month-Day Processed : 10/11/19
Time Processed : 04:46:06 PM
Injection Volume : 0.3
Sample Name : [Tyr1]-MIF-1
Cat No. : RP13116
Lot No. : E557219J
Theoretical MW : 447.53
Observed MW : 447.2

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH