

Sample Name :SV40 large T antigen NLS  
 Cat No. :RP20414  
 Lot No. :PE5101812  
 Time Processed :11:03:53  
 Month-Day-Year Processed :12/11/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	15
25.00	Pumps	Pump A B.Conc	75
25.01	Pumps	Pump A B.Conc	95
30.00	Pumps	Pump A B.Conc	95
30.01	Pumps	Pump A B.Conc	15
40.00	Pumps	Pump A B.Conc	15
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ17010507

<Chromatogram>

mV

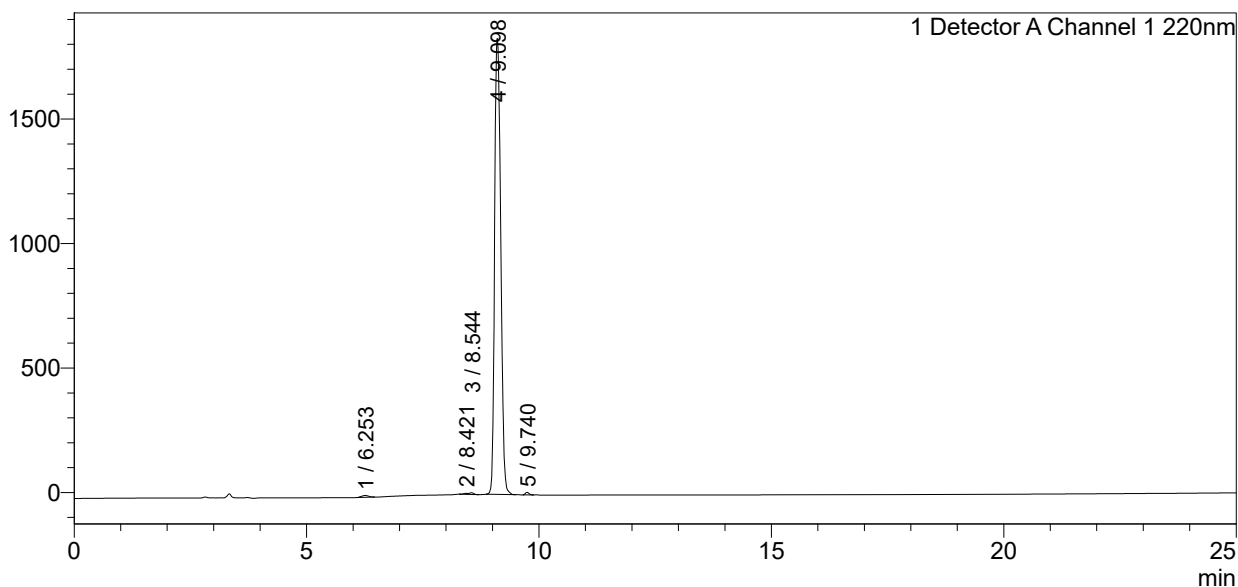

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.253	78715	7425	0.465
2	8.421	17089	4032	0.101
3	8.544	53494	7041	0.316
4	9.098	16732683	1830758	98.793
5	9.740	55215	9788	0.326
Total		16937194	1859044	100.000