

Sample Name :Mycobacterium tuberculosis Protein Ag85A
 Cat. No. :RP20202
 Lot. No. :E6646119H
 Time Processed :7:22:41 AM
 Month-Day-Year Processed :08/14/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

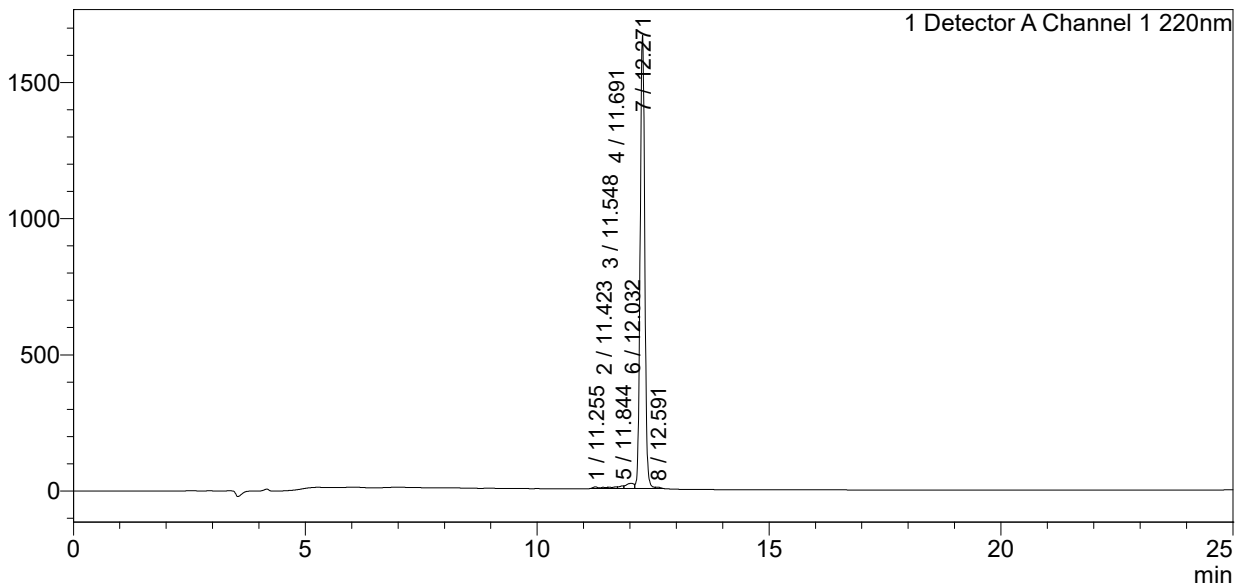

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.255	40132	5660	0.337
2	11.423	37388	4280	0.314
3	11.548	21700	4817	0.182
4	11.691	37200	5558	0.312
5	11.844	62315	9536	0.523
6	12.032	217858	18951	1.829
7	12.271	11460125	1663552	96.215
8	12.591	34283	5001	0.288
Total		11911001	1717355	100.000