

Sample Name : SIYRY  
 Cat. No. : RP20234  
 Lot. No. : PE8711902  
 Time Processed : 5:56:37  
 Month-Day-Year Processed : 03/01/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

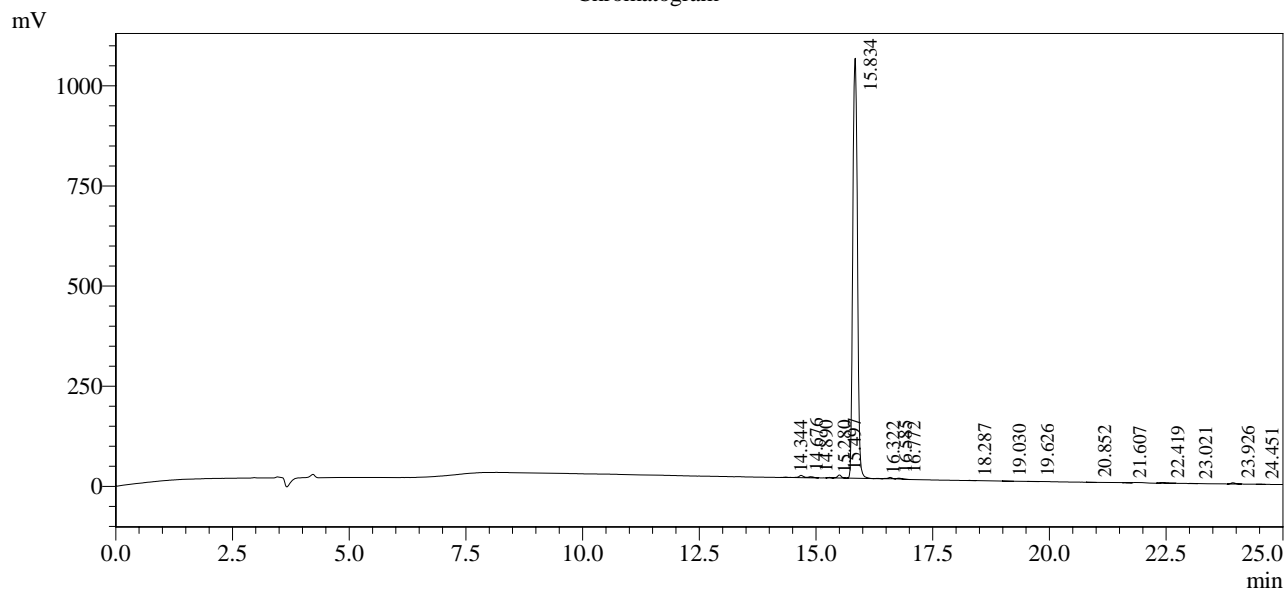

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.344	3831	751	0.051
2	14.676	39336	5551	0.526
3	14.890	20338	2835	0.272
4	15.280	5832	1245	0.078
5	15.497	44955	7623	0.601
6	15.834	7287034	1048723	97.360
7	16.322	3139	552	0.042
8	16.585	20458	3276	0.273
9	16.772	15721	2050	0.210
10	18.287	3163	517	0.042
11	19.030	1046	110	0.014
12	19.626	4126	618	0.055
13	20.852	1179	200	0.016
14	21.607	1073	158	0.014
15	22.419	10034	1284	0.134
16	23.021	1303	205	0.017
17	23.926	20815	3029	0.278
18	24.451	1241	162	0.017
Total		7484623	1078888	100.000