

Sample Name :LAH4
 Cat. No. : RP20096
 Lot. No. : E6075820C
 Time Processed :12:54:24
 Month-Day-Year Processed : 03/27/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

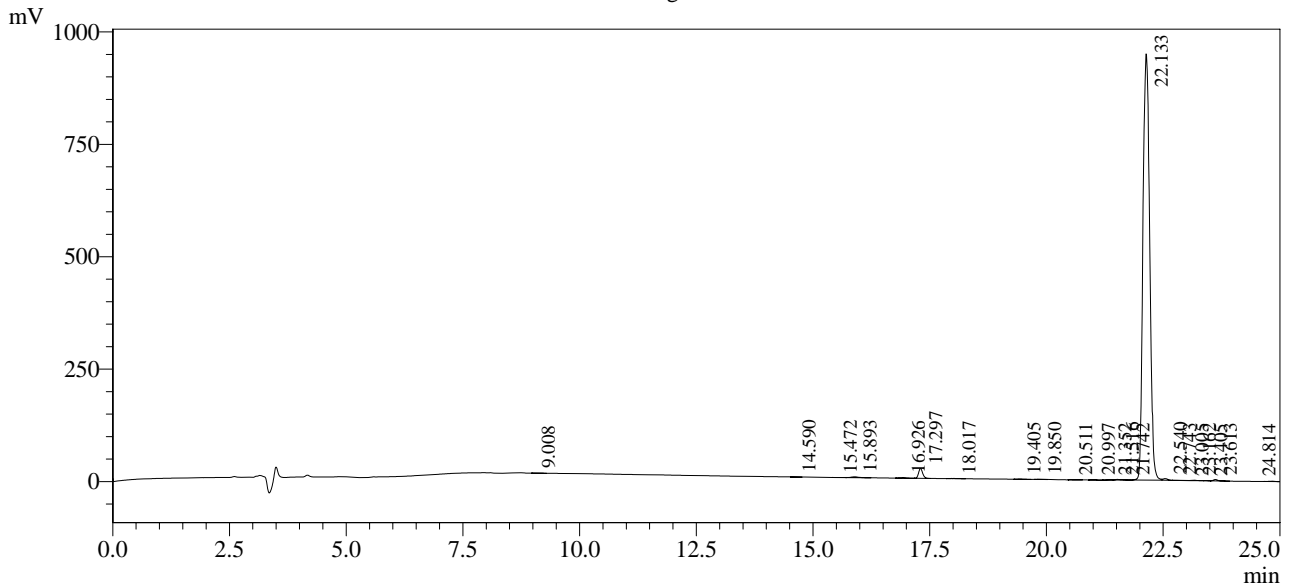

1 Det.A Ch1 / 220nm
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.008	1369	112	0.014
2	14.590	1617	255	0.017
3	15.472	1241	134	0.013
4	15.893	19952	1758	0.204
5	16.926	5501	703	0.056
6	17.297	131840	21989	1.350
7	18.017	5863	405	0.060
8	19.405	4559	385	0.047
9	19.850	7418	960	0.076
10	20.511	1451	142	0.015
11	20.997	2837	452	0.029
12	21.352	2405	328	0.025
13	21.516	10761	1310	0.110
14	21.742	207	61	0.002
15	22.133	9505942	947722	97.329
16	22.540	24224	3663	0.248
17	22.743	1631	331	0.017
18	23.005	2582	450	0.026
19	23.162	5301	838	0.054
20	23.405	1242	291	0.013
21	23.613	22214	3238	0.227
22	24.814	6698	772	0.069
Total		9766854	986298	100.000